

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020625\
 Data File : FG015342.D
 Signal(s) : FID1A.ch
 Acq On : 07 Feb 2025 02:53
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 07 03:19:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG011325.M
 Quant Title :
 QLast Update : Fri Jan 24 12:51:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.043	2217876	17.290 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.225	39231	0.280 ug/ml
13) N-TRIACONTANE	18.116	66925	0.470 ug/ml
14) N-DOTRIACONTANE	18.951	57620	0.415 ug/ml
15) N-TETRATRIACONTANE	19.737	24635	0.197 ug/ml
16) N-HEXATRIACONTANE	20.479	50335	0.466 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020625\
Data File : FG015342.D
Signal(s) : FID1A.ch
Acq On : 07 Feb 2025 02:53
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 07 03:19:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG011325.M
Quant Title :
QLast Update : Fri Jan 24 12:51:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

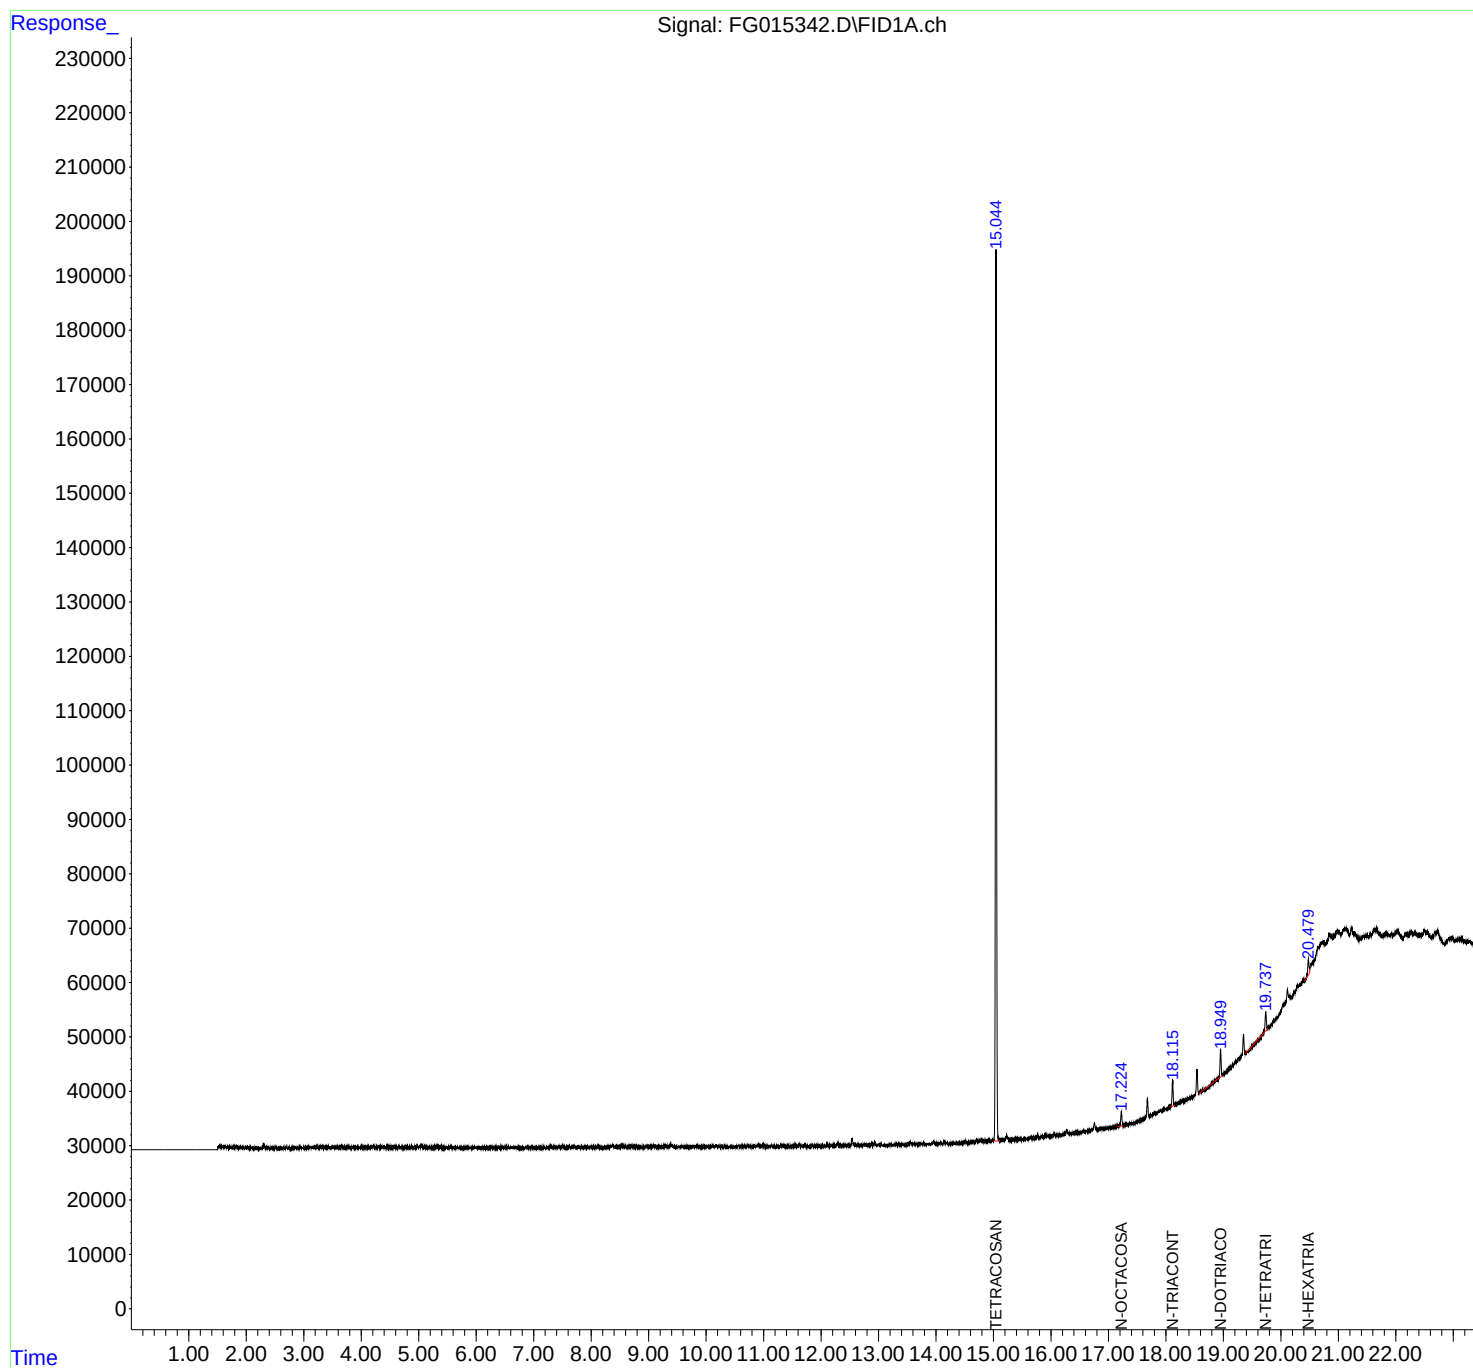


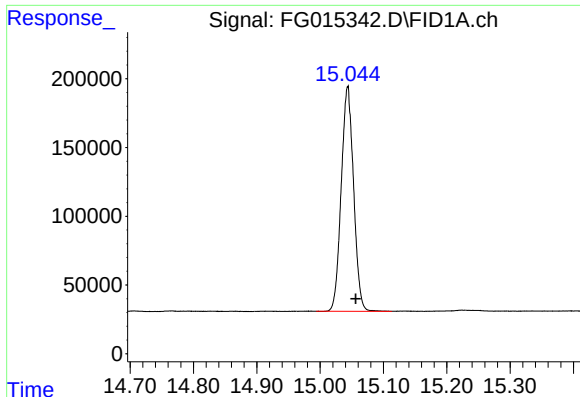

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.043 min
Delta R.T.: -0.013 min
Response: 2217876
Conc: 17.29 ug/ml

Instrument :
FID_G
ClientSampleId :

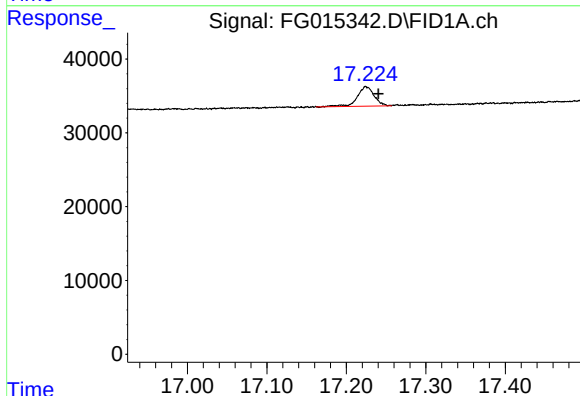


#12 N-OCTACOSANE

R.T.: 17.225 min
Delta R.T.: -0.016 min
Response: 39231
Conc: 0.28 ug/ml

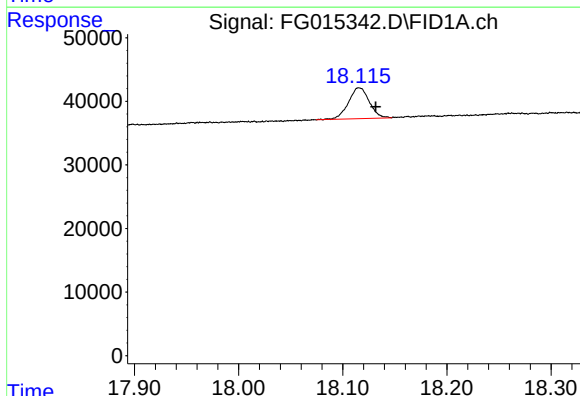


#13 N-TRIACONTANE

R.T.: 18.116 min
Delta R.T.: -0.016 min
Response: 66925
Conc: 0.47 ug/ml

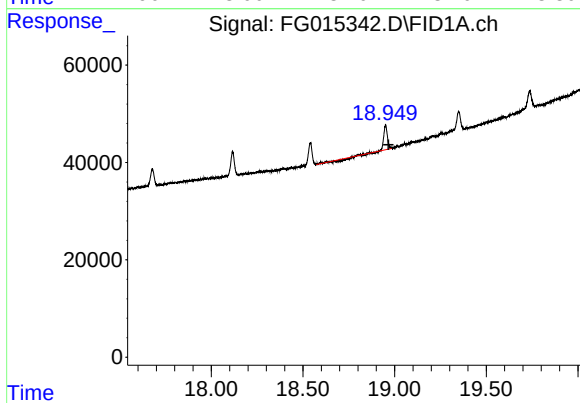

#14 N-DOTRIACONTANE


R.T.: 18.951 min
Delta R.T.: -0.015 min
Response: 57620
Conc: 0.41 ug/ml

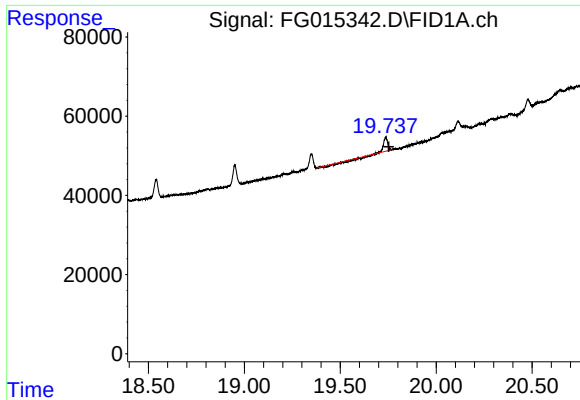

#15 N-TETRATRIACONTANE

R.T.: 19.737 min
Delta R.T.: -0.015 min
Response: 24635
Conc: 0.20 ug/ml

Instrument :
FID_G
ClientSampleId :

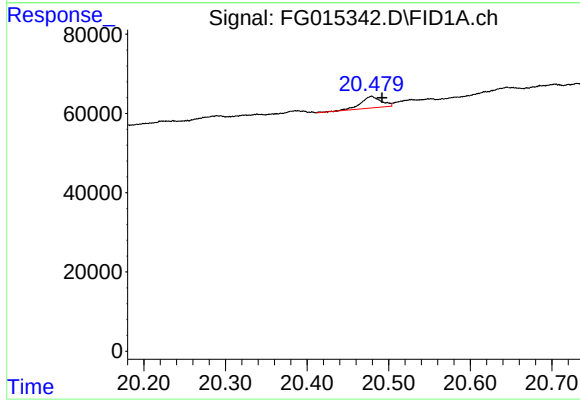

#16 N-HEXATRIACONTANE

R.T.: 20.479 min
Delta R.T.: -0.013 min
Response: 50335
Conc: 0.47 ug/ml