

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG020719\
 Data File : FG003722.D
 Signal(s) : FID1A.ch
 Acq On : 08 Feb 2019 04:56
 Operator : AJ\SJ
 Sample : K1392-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 08 08:14:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.462	1848917	13.670 ug/ml
Target Compounds			
2) N-DECANE	4.197	11009437	69.801 ug/ml
3) N-DODECANE	6.216	3126280	19.801 ug/ml
4) N-TETRADECANE	8.012	4189989	26.547 ug/ml
5) N-HEXADECANE	9.614	2793652	17.734 ug/ml
6) N-OCTADECANE	11.056	4978007	31.623 ug/ml
7) N-EICOSANE	12.368	3876614	24.752 ug/ml
12) N-OCTACOSANE	16.637	387900	2.692 ug/ml
13) N-TRIACONTANE	17.525	462897	3.271 ug/ml
14) N-DOTRIACONTANE	18.357	424254	3.240 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG020719\
Data File : FG003722.D
Signal(s) : FID1A.ch
Acq On : 08 Feb 2019 04:56
Operator : AJ\SJ
Sample : K1392-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 08:14:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

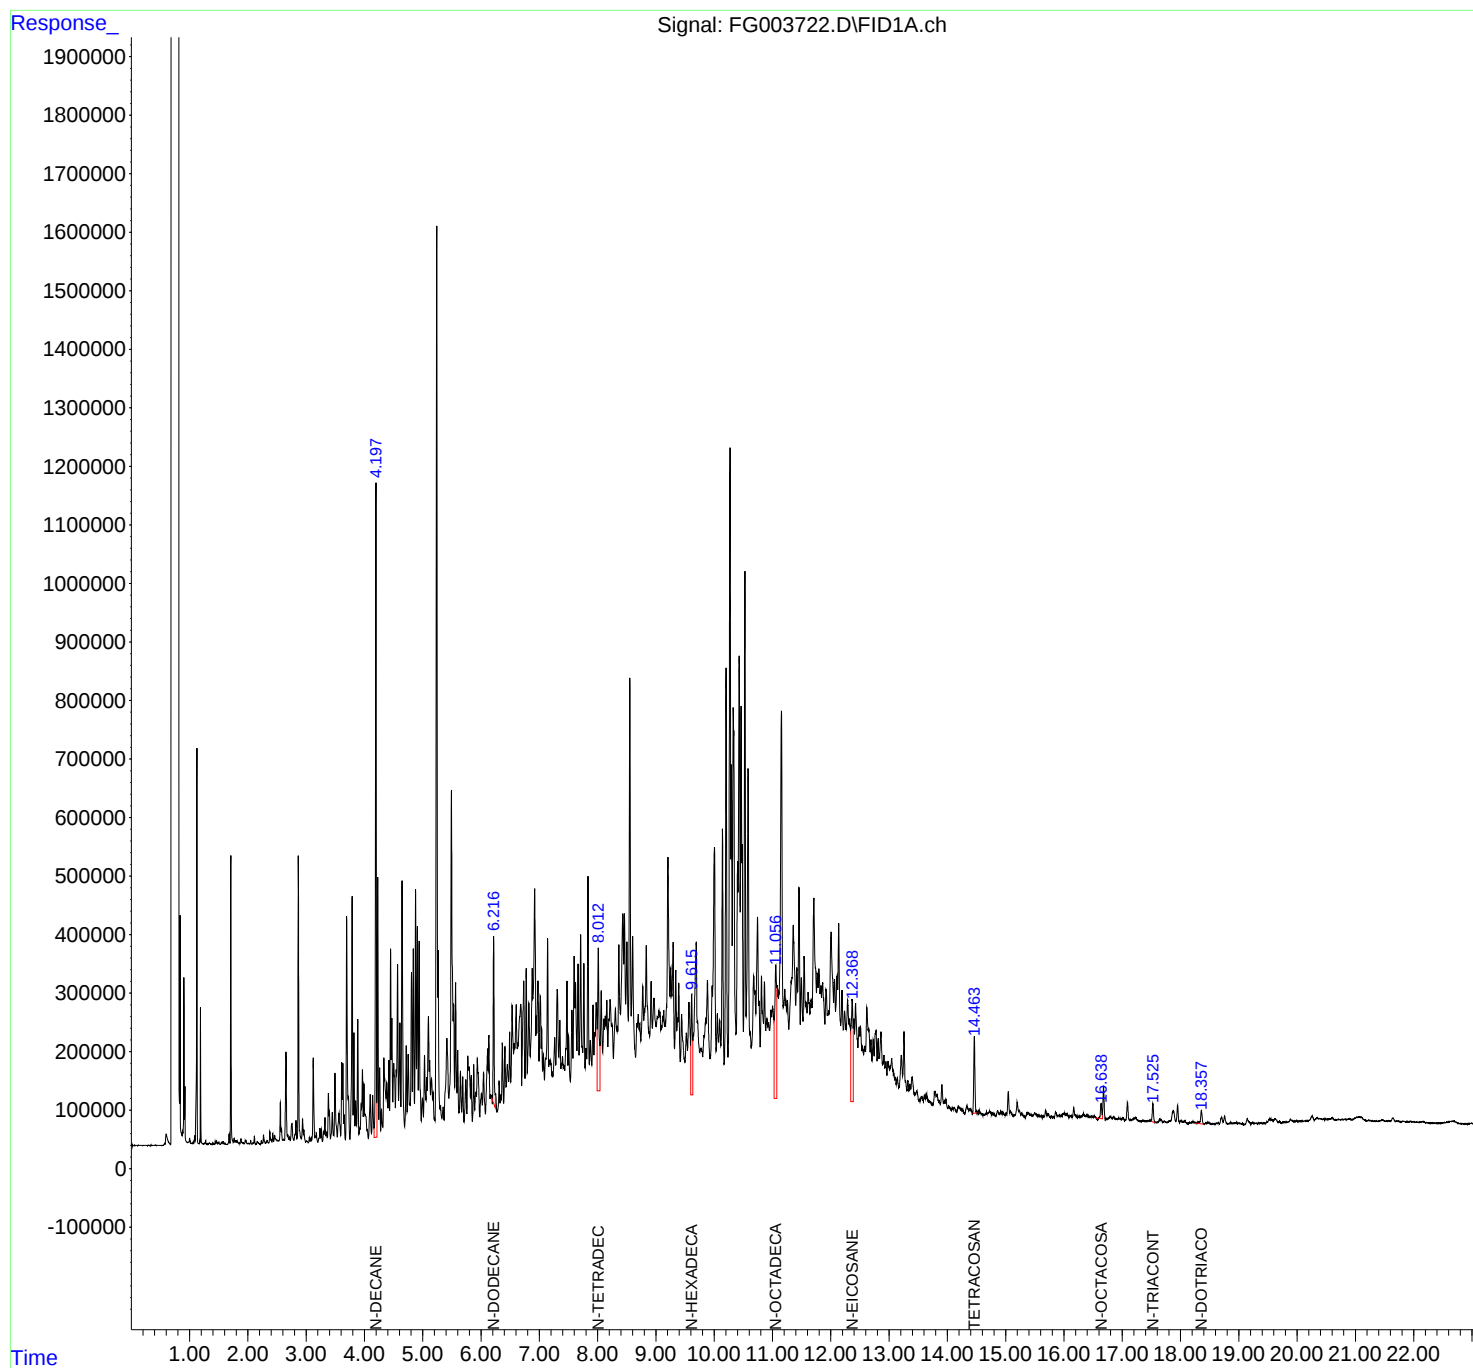

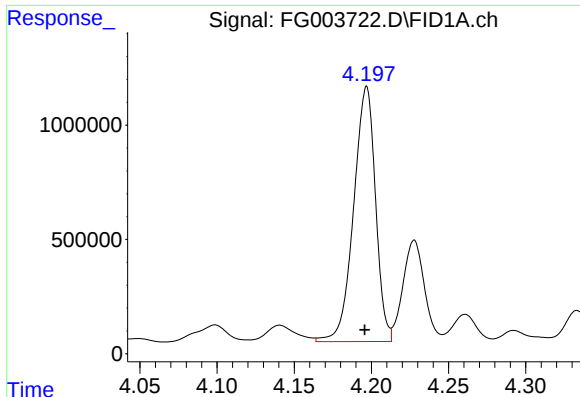


#2 N-DECANE

R.T.: 4.197 min
Delta R.T.: 0.001 min
Response: 11009437
Conc: 69.80 ug/ml

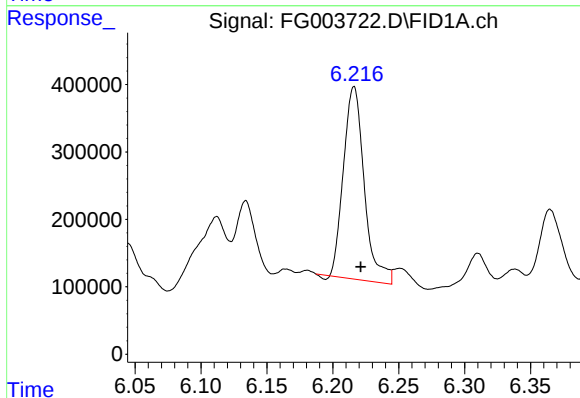


#3 N-DODECANE

R.T.: 6.216 min
Delta R.T.: -0.005 min
Response: 3126280
Conc: 19.80 ug/ml

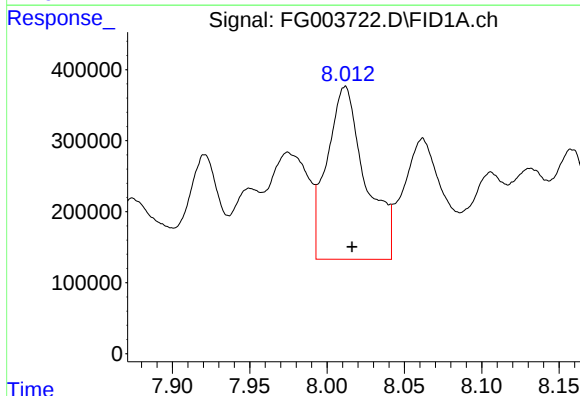


#4 N-TETRADECANE

R.T.: 8.012 min
Delta R.T.: -0.004 min
Response: 4189989
Conc: 26.55 ug/ml

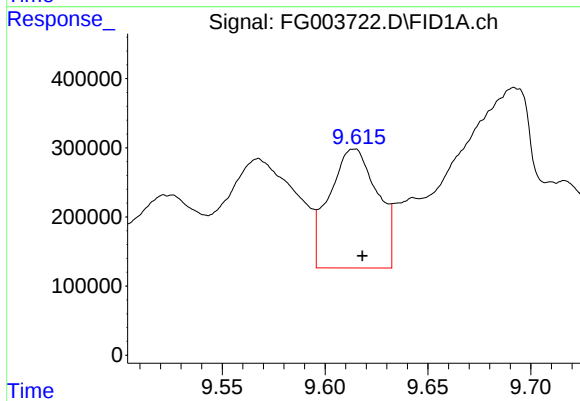


#5 N-HEXADECANE

R.T.: 9.614 min
Delta R.T.: -0.004 min
Response: 2793652
Conc: 17.73 ug/ml

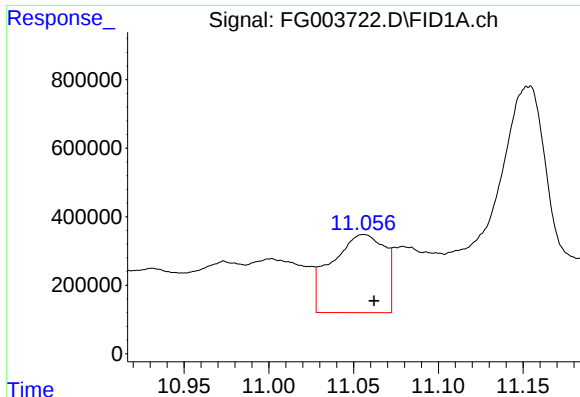


#6 N-OCTADECANE

R.T.: 11.056 min
Delta R.T.: -0.006 min
Response: 4978007
Conc: 31.62 ug/ml

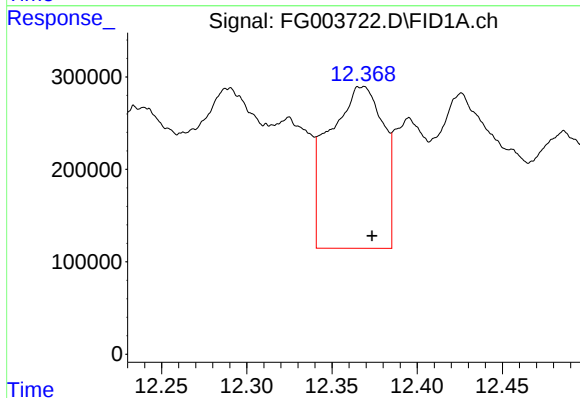


#7 N-EICOSANE

R.T.: 12.368 min
Delta R.T.: -0.005 min
Response: 3876614
Conc: 24.75 ug/ml

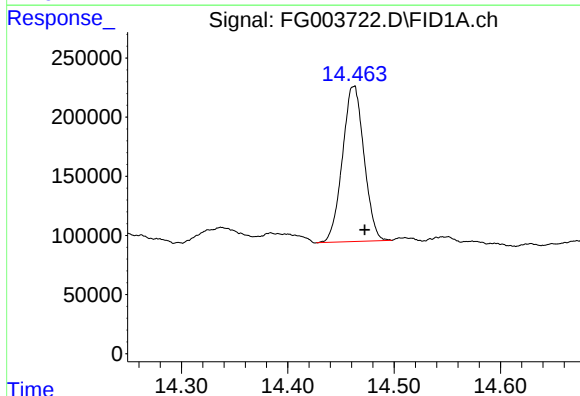


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.462 min
Delta R.T.: -0.010 min
Response: 1848917
Conc: 13.67 ug/ml

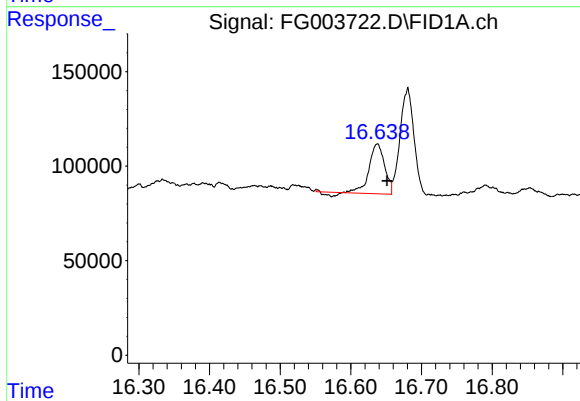


#12 N-OCTACOSANE

R.T.: 16.637 min
Delta R.T.: -0.014 min
Response: 387900
Conc: 2.69 ug/ml

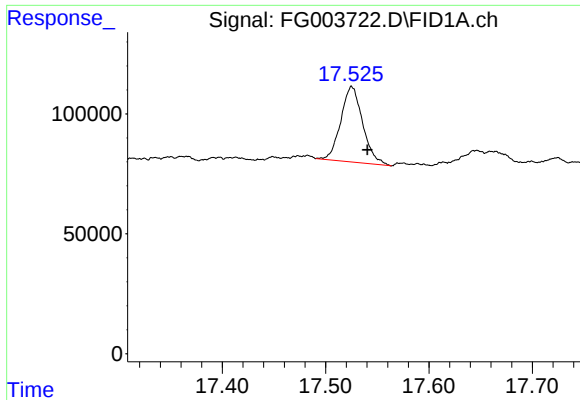

#13 N-TRIACONTANE

R.T.: 17.525 min
Delta R.T.: -0.015 min
Response: 462897
Conc: 3.27 ug/ml

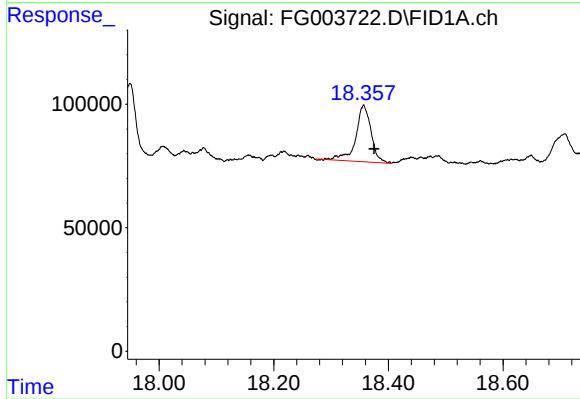

#14 N-DOTRIACONTANE

R.T.: 18.357 min
Delta R.T.: -0.018 min
Response: 424254
Conc: 3.24 ug/ml