

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020720\
 Data File : FG006629.D
 Signal(s) : FID1A.ch
 Acq On : 07 Feb 2020 13:16
 Operator : DD\AJ
 Sample : L1433-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 07 23:04:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG012820.M
 Quant Title :
 QLast Update : Wed Jan 29 08:10:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	1429714	15.247 ug/ml
Target Compounds			
7) N-EICOSANE	12.530	90876	0.831 ug/ml
8) N-DOCOSANE	13.695	173471	1.598 ug/ml
10) N-TETRACOSANE	14.774	84890	0.786 ug/ml
11) N-HEXACOSANE	15.798	105223	0.977 ug/ml
12) N-OCTACOSANE	16.716	724123	6.474 ug/ml
13) N-TRIACONTANE	17.589	184009	1.551 ug/ml
14) N-DOTRIACONTANE	18.399	305003	2.792 ug/ml
16) N-HEXATRIACONTANE	19.879	355324	3.630 ug/ml
18) N-TETRACONTANE	21.328	252601	2.843 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020720\
Data File : FG006629.D
Signal(s) : FID1A.ch
Acq On : 07 Feb 2020 13:16
Operator : DD\AJ
Sample : L1433-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Feb 07 23:04:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG012820.M
Quant Title :
QLast Update : Wed Jan 29 08:10:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

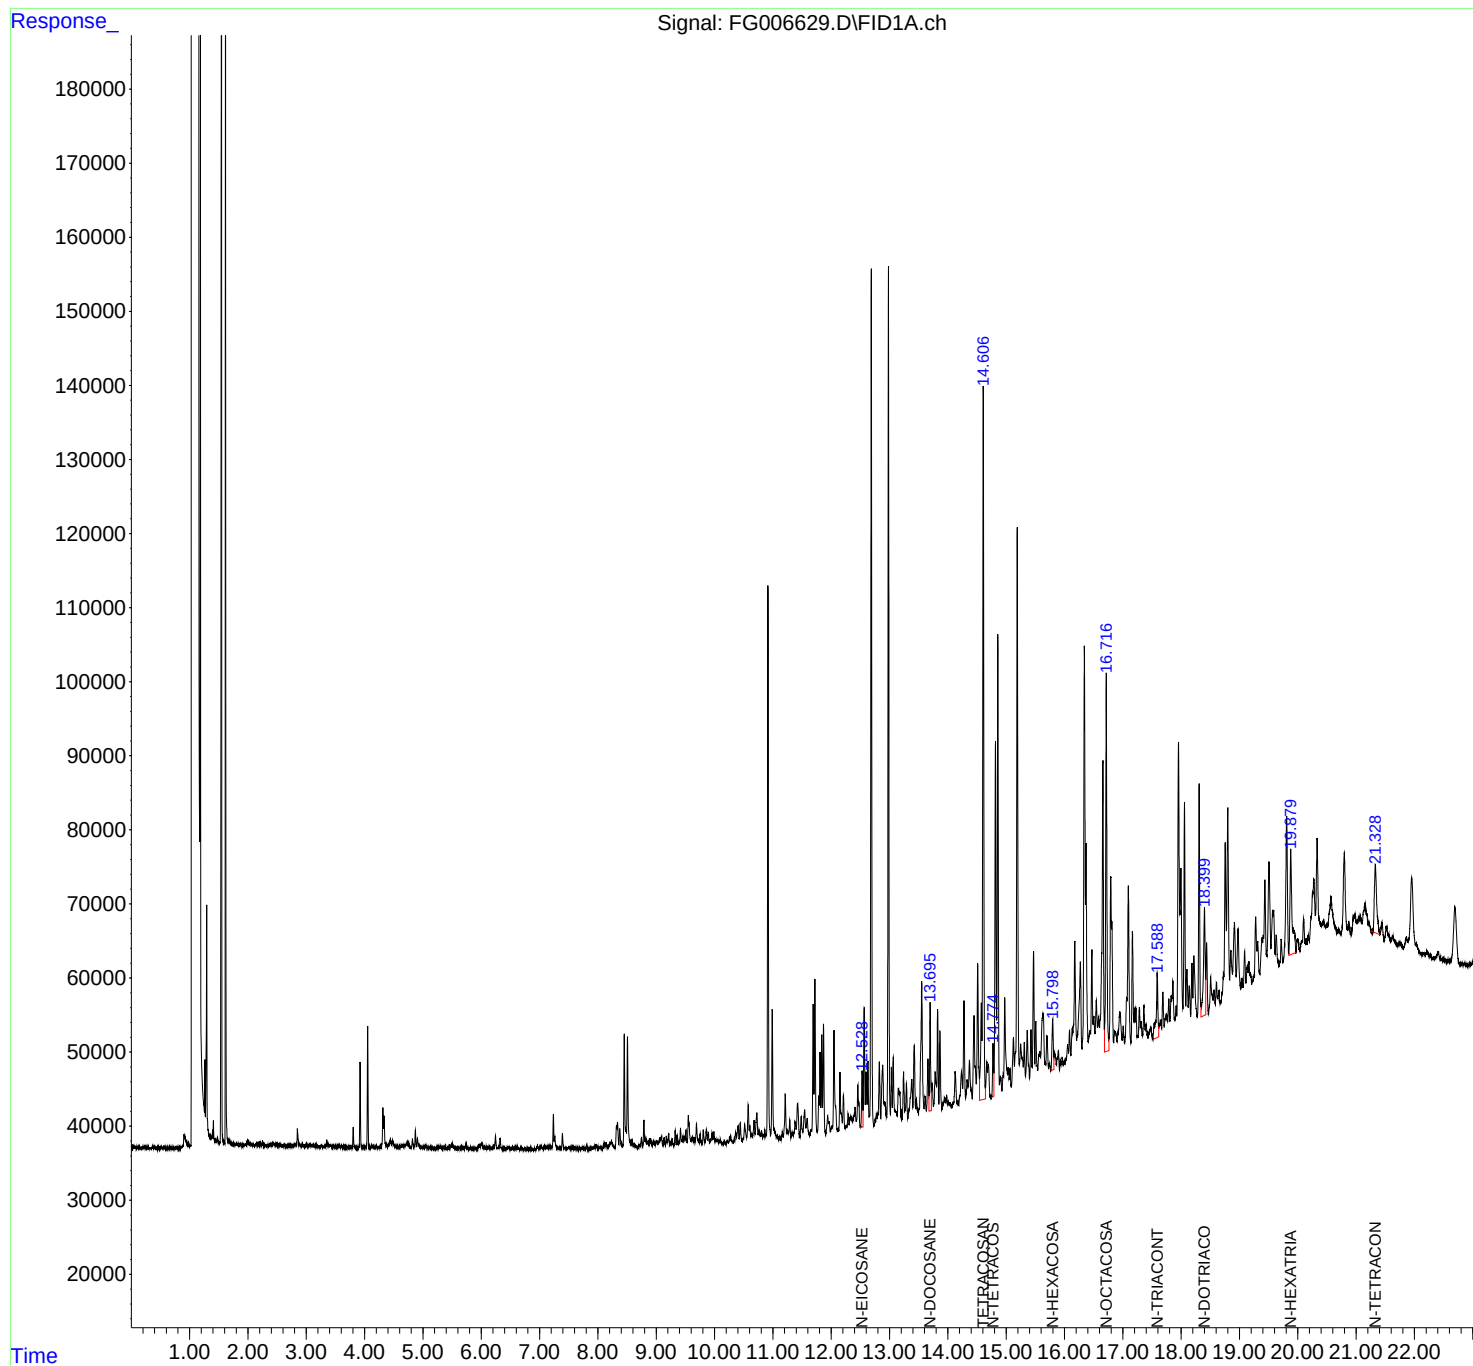


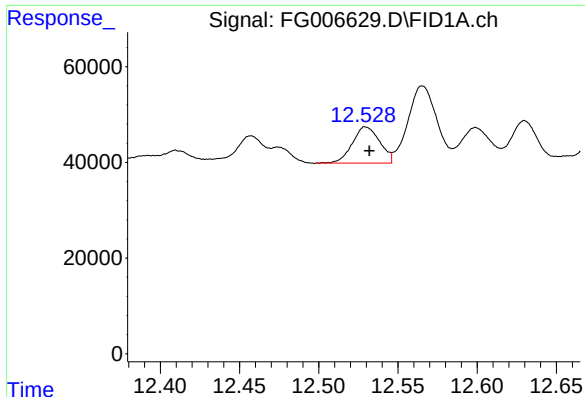

#7 N-EICOSANE


R.T.: 12.530 min
Delta R.T.: -0.002 min
Response: 90876
Conc: 0.83 ug/ml

Instrument :
FID_G
ClientSampleId :

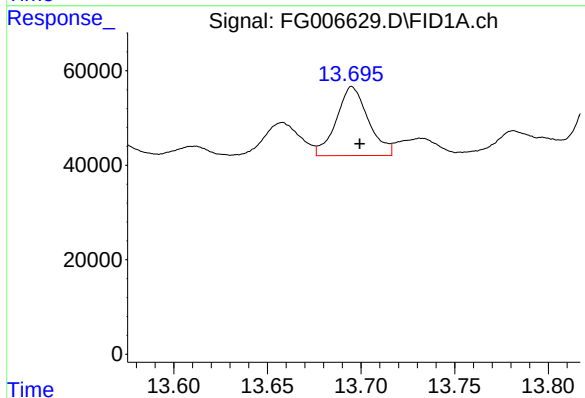


#8 N-DOCOSANE

R.T.: 13.695 min
Delta R.T.: -0.004 min
Response: 173471
Conc: 1.60 ug/ml

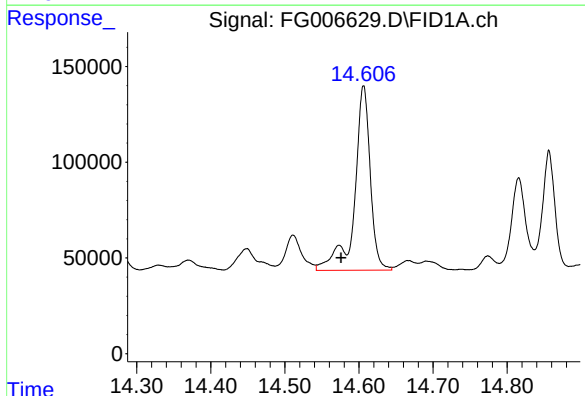


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.606 min
Delta R.T.: 0.031 min
Response: 1429714
Conc: 15.25 ug/ml

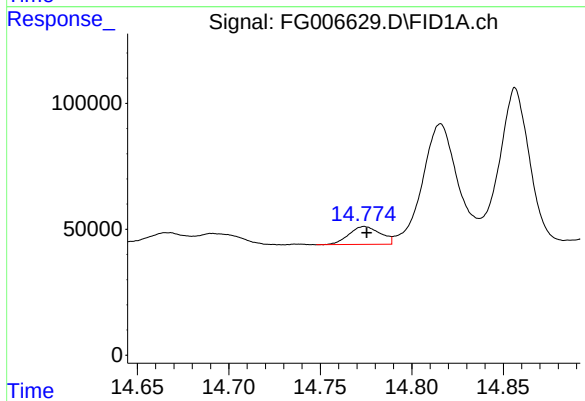

#10 N-TETRACOSANE


R.T.: 14.774 min
Delta R.T.: 0.000 min
Response: 84890
Conc: 0.79 ug/ml

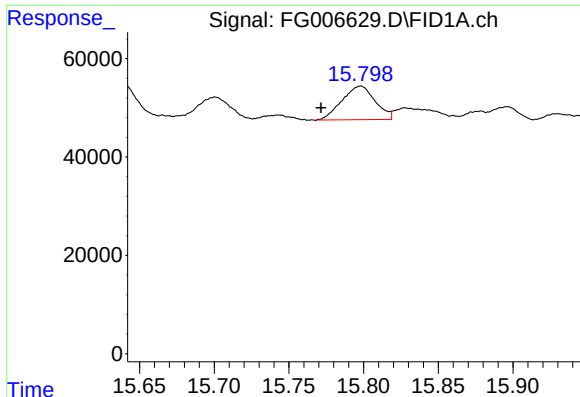

#11 N-HEXACOSANE


R.T.: 15.798 min
Delta R.T.: 0.026 min
Response: 105223
Conc: 0.98 ug/ml

Instrument :
FID_G
ClientSampleId :

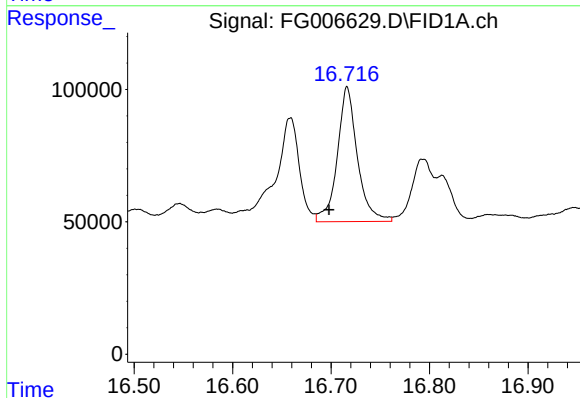


#12 N-OCTACOSANE

R.T.: 16.716 min
Delta R.T.: 0.019 min
Response: 724123
Conc: 6.47 ug/ml

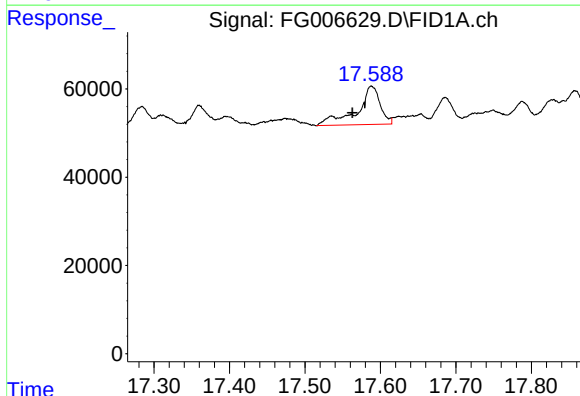


#13 N-TRIACONTANE

R.T.: 17.589 min
Delta R.T.: 0.026 min
Response: 184009
Conc: 1.55 ug/ml

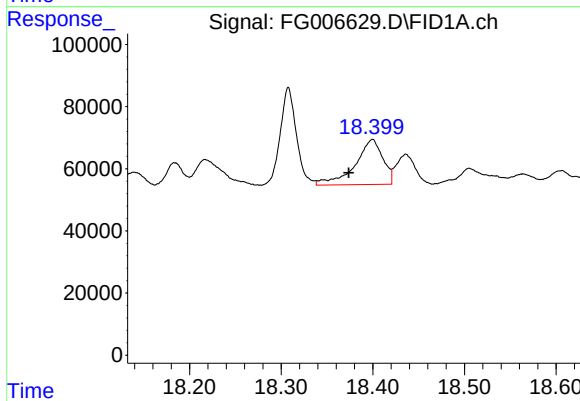

#14 N-DOTRIACONTANE


R.T.: 18.399 min
Delta R.T.: 0.026 min
Response: 305003
Conc: 2.79 ug/ml

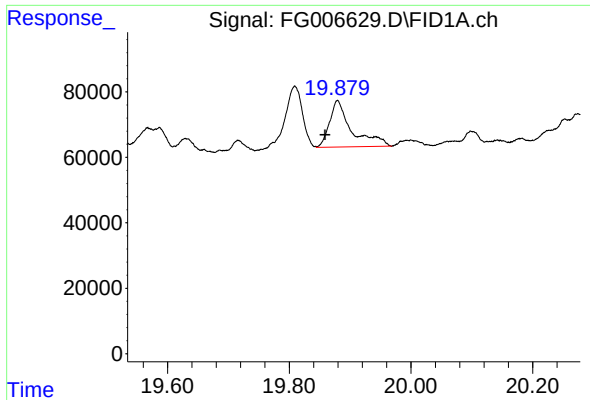

#16 N-HEXATRIACONTANE

R.T.: 19.879 min
Delta R.T.: 0.020 min
Response: 355324
Conc: 3.63 ug/ml

Instrument :
FID_G
ClientSampleId :

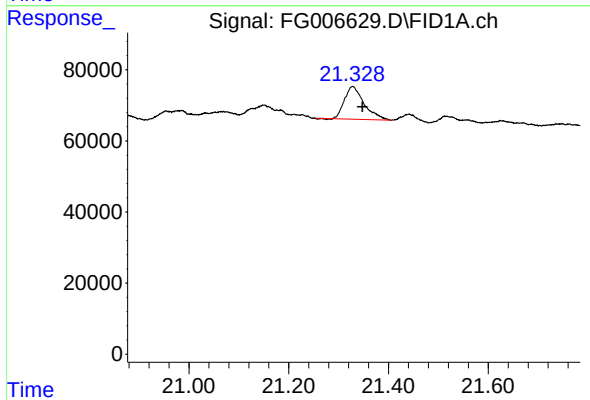

#18 N-TETRACONTANE

R.T.: 21.328 min
Delta R.T.: -0.020 min
Response: 252601
Conc: 2.84 ug/ml