

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020720\
 Data File : FG006641.D
 Signal(s) : FID1A.ch
 Acq On : 07 Feb 2020 19:23
 Operator : DD\AJ
 Sample : L1439-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 07 23:22:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG012820.M
 Quant Title :
 QLast Update : Wed Jan 29 08:10:21 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	1399284	14.922 ug/ml
Target Compounds			
6) N-OCTADECANE	11.214	106166	0.989 ug/ml
7) N-EICOSANE	12.568	150246	1.374 ug/ml
8) N-DOCOSANE	13.697	131585	1.212 ug/ml
10) N-TETRACOSANE	14.816	876628	8.118 ug/ml
11) N-HEXACOSANE	15.794	100925	0.937 ug/ml
12) N-OCTACOSANE	16.716	865339	7.736 ug/ml
13) N-TRIACONTANE	17.588	82510	0.695 ug/ml
14) N-DOTRIACONTANE	18.394	280241	2.565 ug/ml
16) N-HEXATRIACONTANE	19.875	354054	3.617 ug/ml
18) N-TETRACONTANE	21.325	290727	3.272 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020720\
Data File : FG006641.D
Signal(s) : FID1A.ch
Acq On : 07 Feb 2020 19:23
Operator : DD\AJ
Sample : L1439-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 07 23:22:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG012820.M
Quant Title :
QLast Update : Wed Jan 29 08:10:21 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

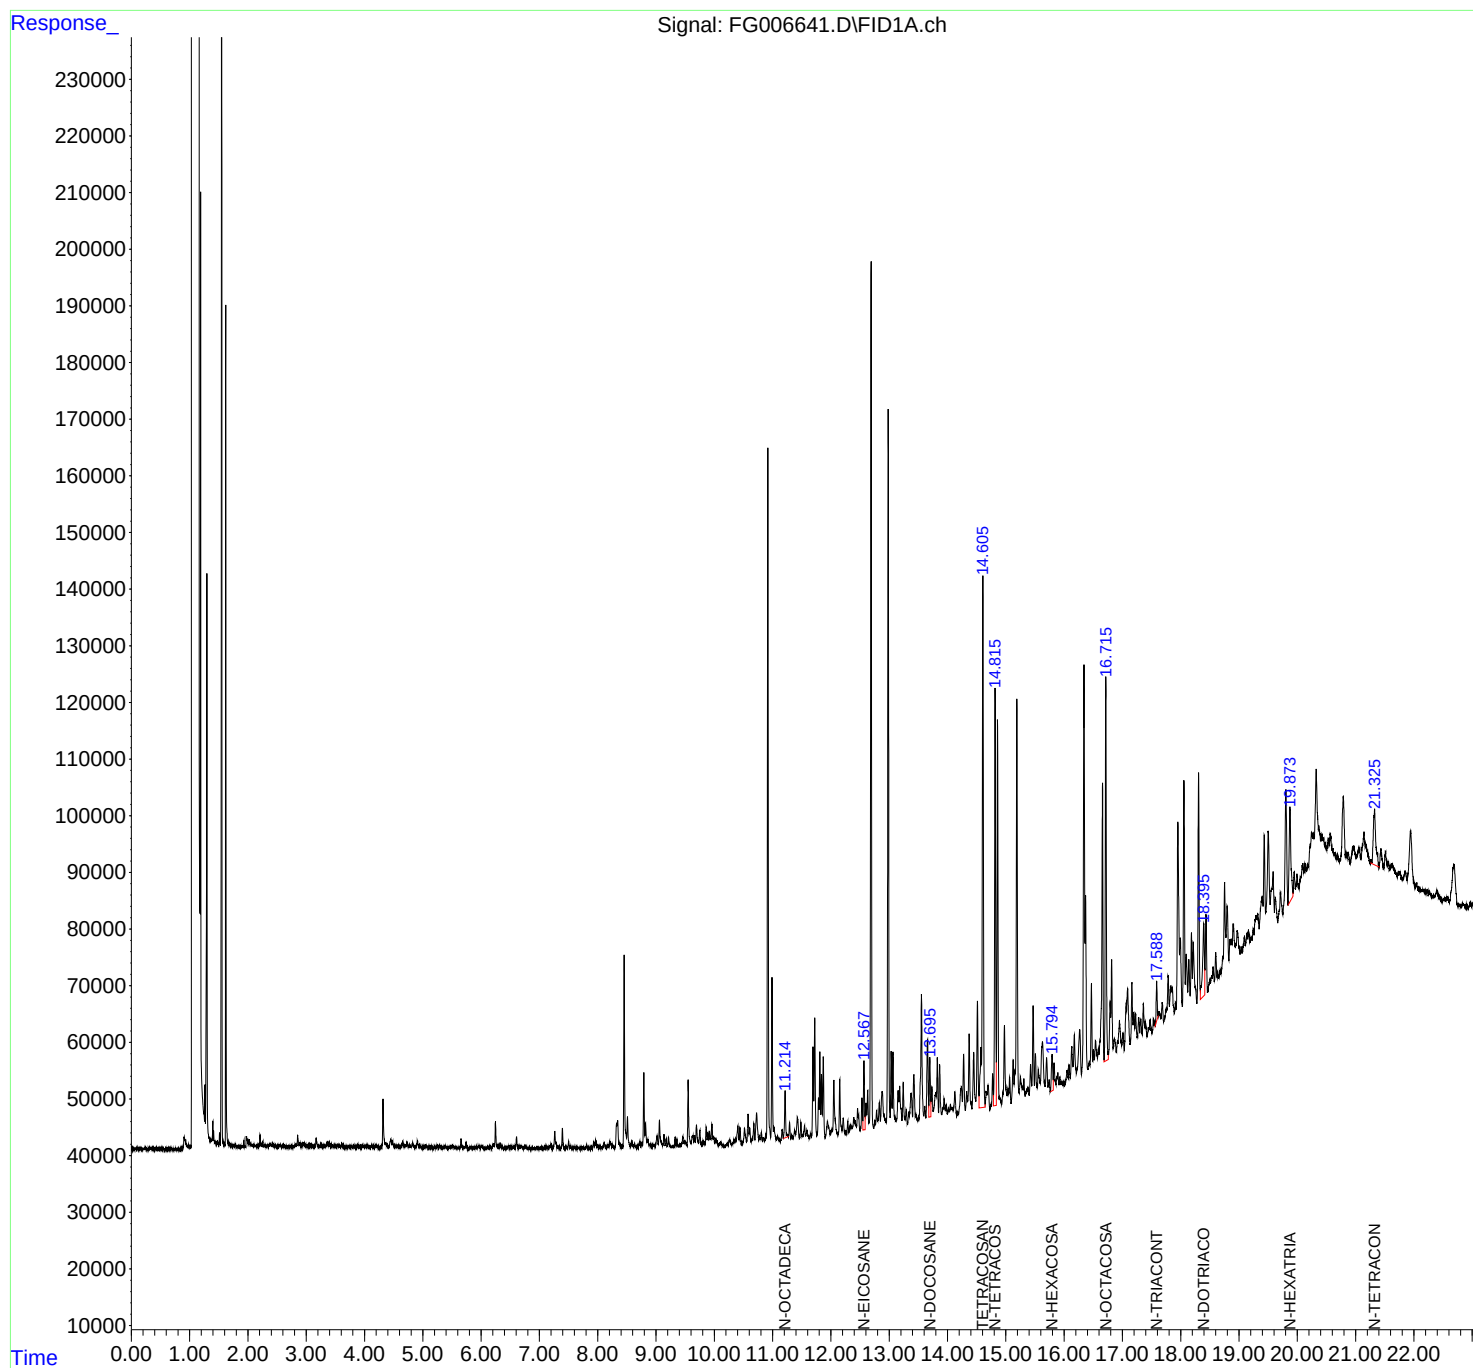


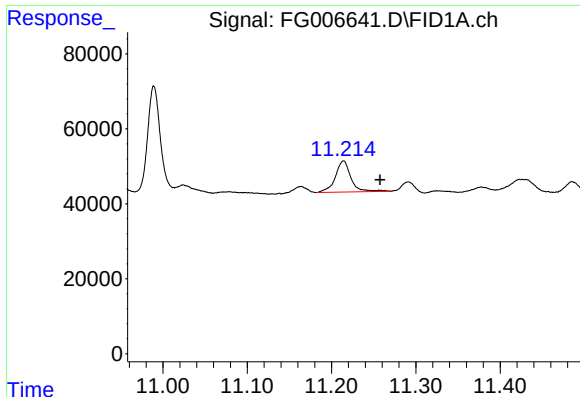

#6 N-OCTADECANE


R.T.: 11.214 min
Delta R.T.: -0.044 min
Response: 106166
Conc: 0.99 ug/ml

Instrument :
FID_G
ClientSampleId :

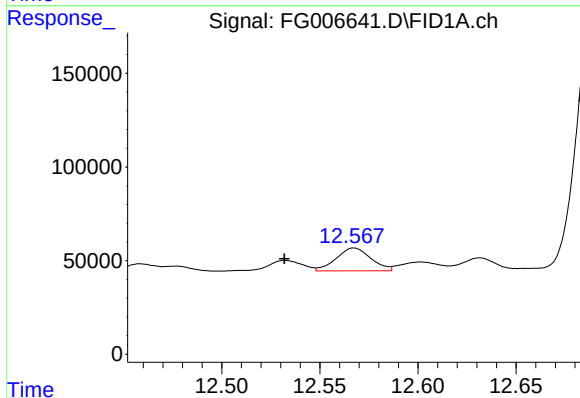


#7 N-EICOSANE

R.T.: 12.568 min
Delta R.T.: 0.036 min
Response: 150246
Conc: 1.37 ug/ml

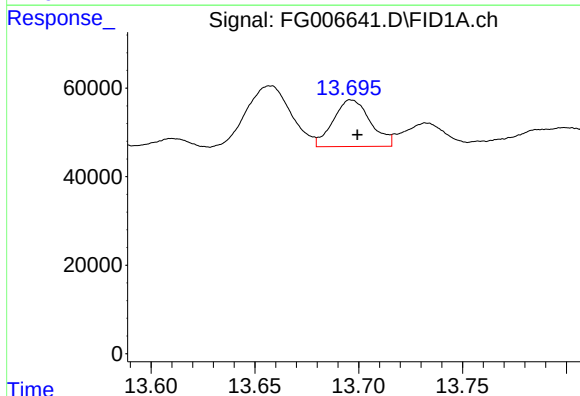


#8 N-DOCOSANE

R.T.: 13.697 min
Delta R.T.: -0.003 min
Response: 131585
Conc: 1.21 ug/ml

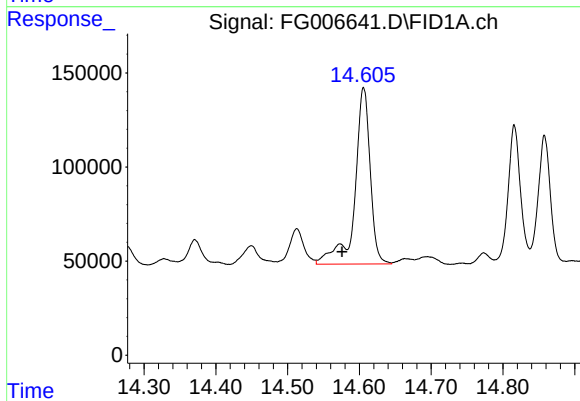

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.606 min
Delta R.T.: 0.030 min
Response: 1399284
Conc: 14.92 ug/ml

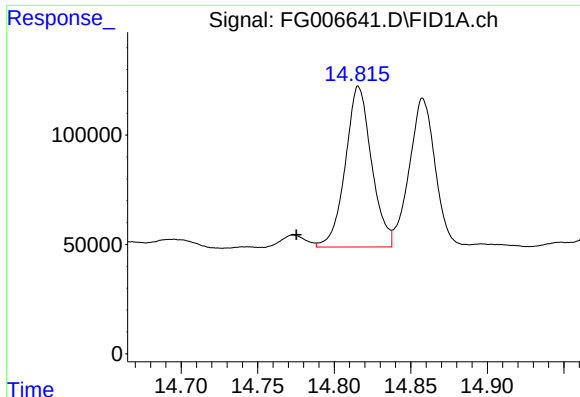

#10 N-TETRACOSANE


R.T.: 14.816 min
Delta R.T.: 0.041 min
Response: 876628
Conc: 8.12 ug/ml

Instrument :
FID_G
ClientSampleId :

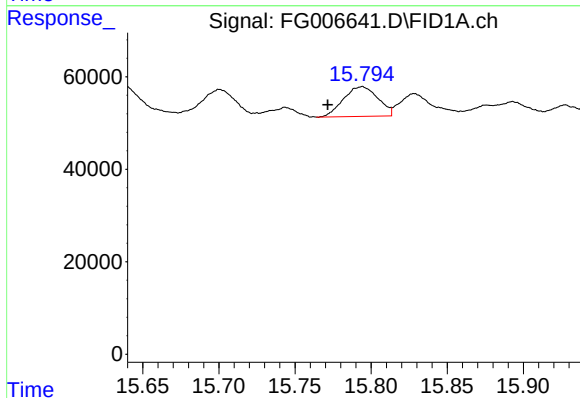


#11 N-HEXACOSANE

R.T.: 15.794 min
Delta R.T.: 0.022 min
Response: 100925
Conc: 0.94 ug/ml

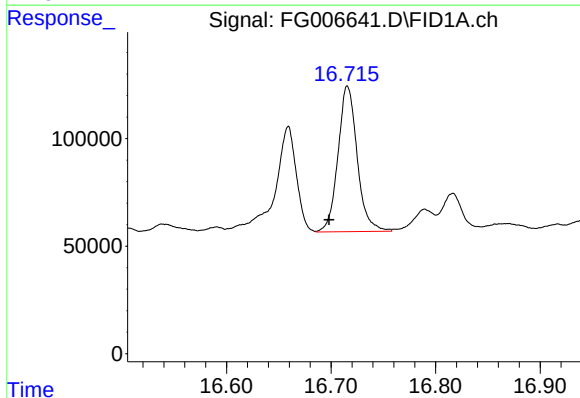


#12 N-OCTACOSANE

R.T.: 16.716 min
Delta R.T.: 0.018 min
Response: 865339
Conc: 7.74 ug/ml

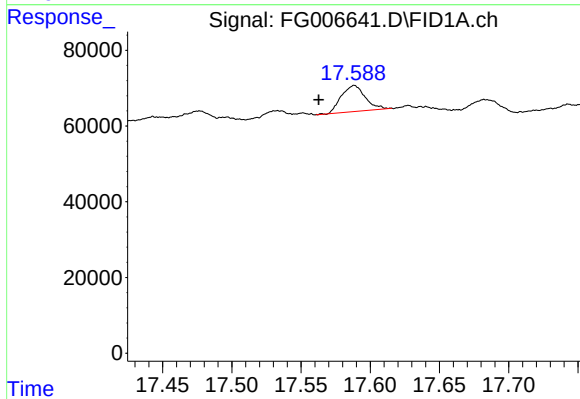

#13 N-TRIACONTANE


R.T.: 17.588 min
Delta R.T.: 0.025 min
Response: 82510
Conc: 0.70 ug/ml

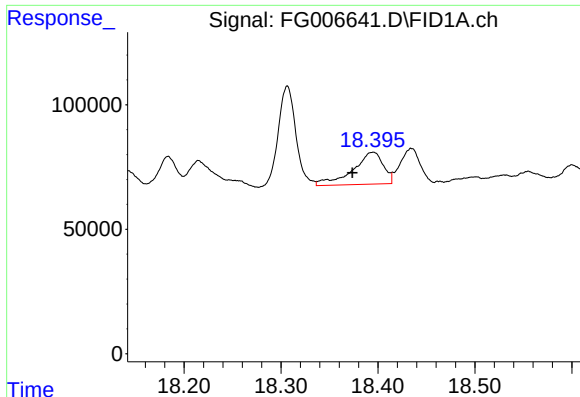

#14 N-DOTRIACONTANE


R.T.: 18.394 min
Delta R.T.: 0.021 min
Response: 280241
Conc: 2.57 ug/ml

Instrument :
FID_G
ClientSampleId :

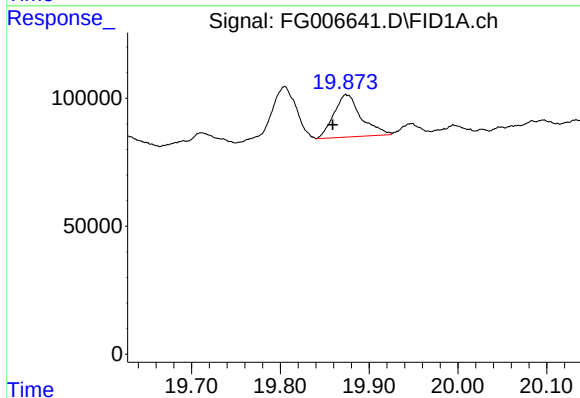

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.016 min
Response: 354054
Conc: 3.62 ug/ml

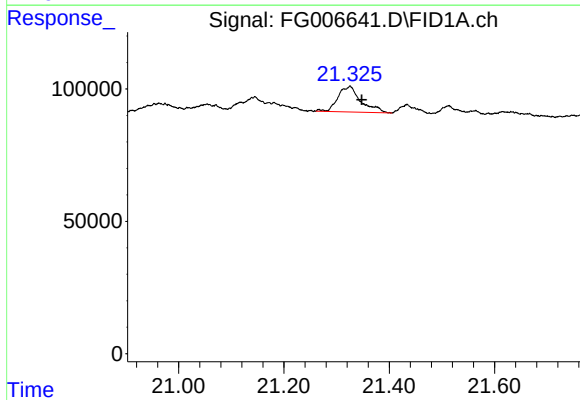

#18 N-TETRACONTANE

R.T.: 21.325 min
Delta R.T.: -0.023 min
Response: 290727
Conc: 3.27 ug/ml