

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG020720\  
Data File : FG006648.D  
Signal(s) : FID1A.ch  
Acq On : 07 Feb 2020 22:54  
Operator : DD\AJ  
Sample : L1438-03  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
HAM-WC-S-SB-0203

Manual Integrations  
APPROVED

Sohil  
2/10/2020 11:41:21 AM

Integration File: autoint1.e  
Quant Time: Feb 07 23:24:41 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG012820.M  
Quant Title :  
QLast Update : Wed Jan 29 08:10:21 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.622 | 2171437  | 23.157 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG020720\  
Data File : FG006648.D  
Signal(s) : FID1A.ch  
Acq On : 07 Feb 2020 22:54  
Operator : DD\AJ  
Sample : L1438-03  
Misc :  
ALS Vial : 21 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
HAM-WC-S-SB-0203


Manual Integrations  
APPROVED

Sohil  
2/10/2020 11:41:21 AM

Integration File: autoint1.e  
Quant Time: Feb 07 23:24:41 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG012820.M  
Quant Title :  
QLast Update : Wed Jan 29 08:10:21 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

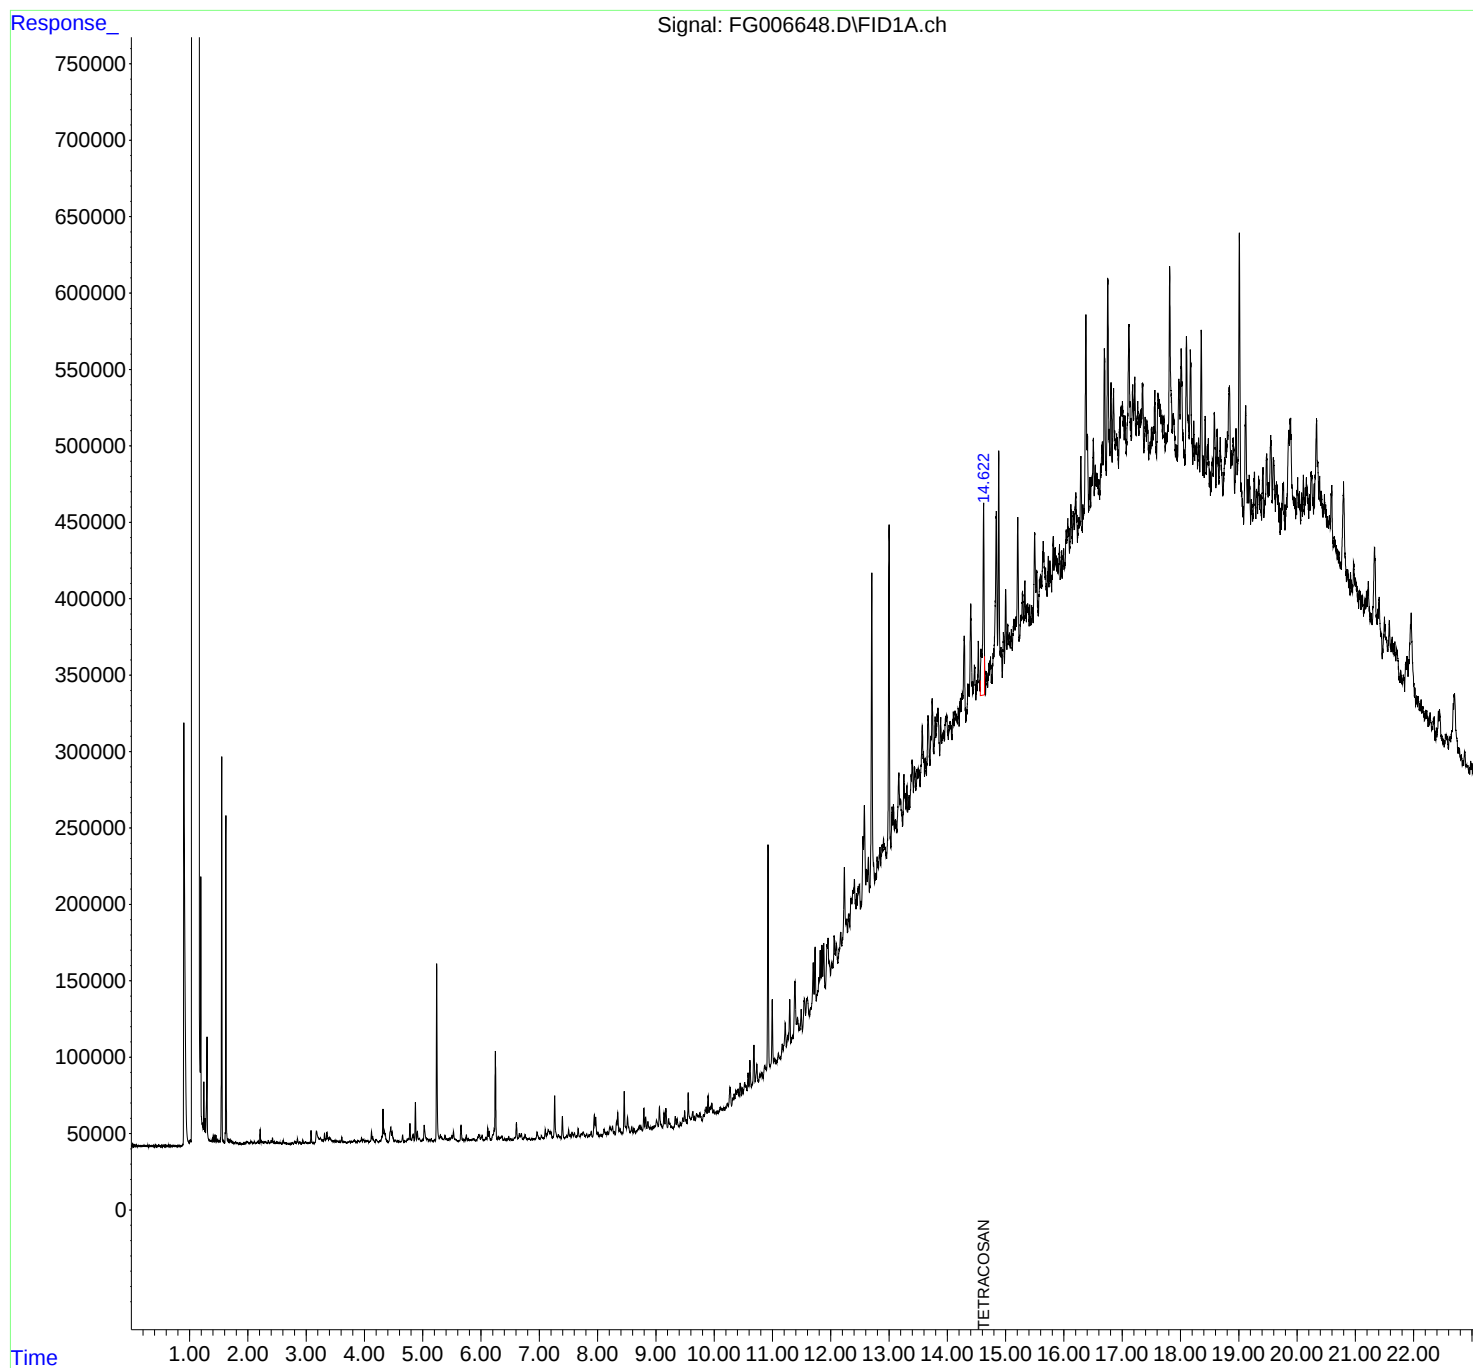

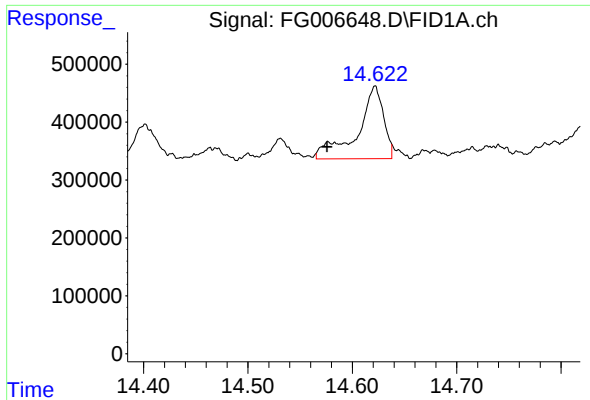

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.622 min  
Delta R.T.: 0.046 min  
Response: 2171437  
Conc: 23.16 ug/ml m

Instrument :  
FID\_G  
ClientSampleId :  
HAM-WC-S-SB-0203

Manual Integrations  
APPROVED

Sohil  
2/10/2020 11:41:21 AM