

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020724\
Data File : FG013480.D
Signal(s) : FID1A.ch
Acq On : 07 Feb 2024 10:55
Operator : YP\AJ
Sample : PB158753BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 02:42:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020124.M
Quant Title :
QLast Update : Thu Feb 01 14:07:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.070	2409545	21.522 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.977	50621	0.485 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020724\
Data File : FG013480.D
Signal(s) : FID1A.ch
Acq On : 07 Feb 2024 10:55
Operator : YP\AJ
Sample : PB158753BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 02:42:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020124.M
Quant Title :
QLast Update : Thu Feb 01 14:07:32 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

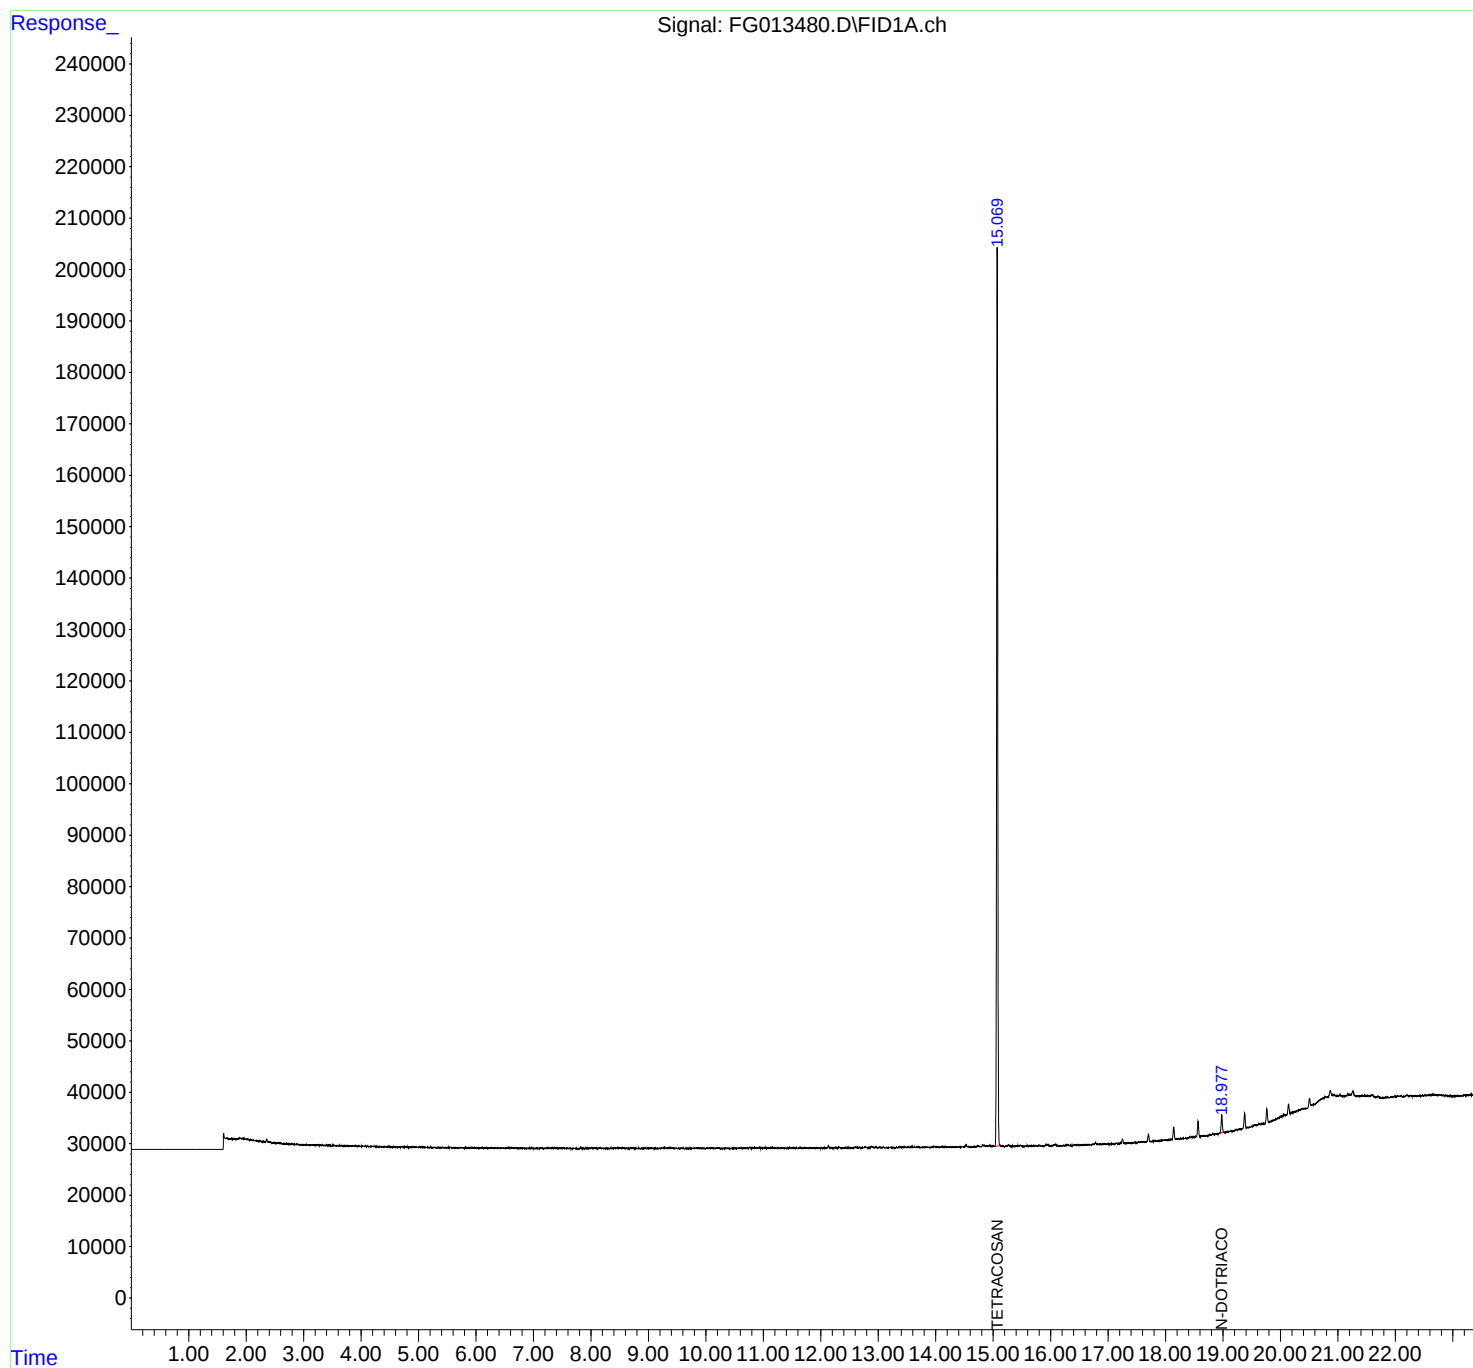

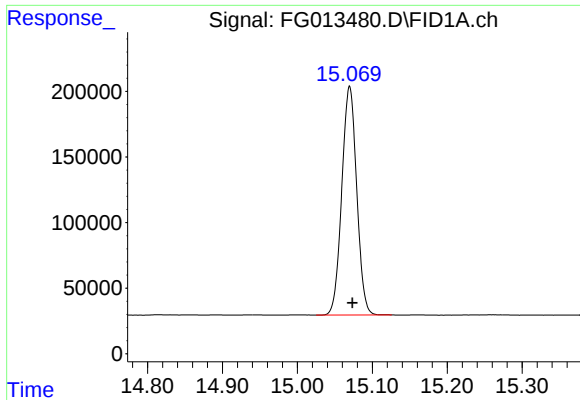

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.070 min
Delta R.T.: -0.004 min
Response: 2409545
Conc: 21.52 ug/ml

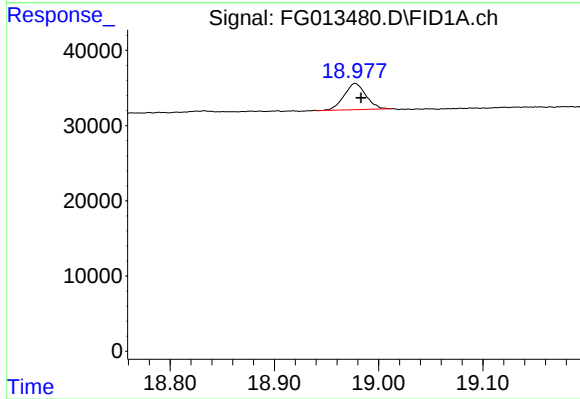

#14 N-DOTRIACONTANE

R.T.: 18.977 min
Delta R.T.: -0.006 min
Response: 50621
Conc: 0.48 ug/ml