

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020819\
 Data File : FG003734.D
 Signal(s) : FID1A.ch
 Acq On : 08 Feb 2019 13:34
 Operator : AJ\SJ
 Sample : K1389-06 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 08 22:44:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.464	743709	5.499 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.065	151003	0.957 ug/ml
7)	N-EICOSANE	12.402	933436	5.960 ug/ml
10)	N-TETRACOSANE	14.623f	478262	3.174 ug/ml
12)	N-OCTACOSANE	16.640	481875	3.345 ug/ml
13)	N-TRIACONTANE	17.530	506051	3.576 ug/ml
14)	N-DOTRIACONTANE	18.363	301978	2.306 ug/ml
15)	N-TETRATRIACONTANE	19.149	437657	3.711 ug/ml
16)	N-HEXATRIACONTANE	19.898	191680	1.816 ug/ml
17)	N-OCTATRIACONTANE	20.616	495891	5.072 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG020819\
Data File : FG003734.D
Signal(s) : FID1A.ch
Acq On : 08 Feb 2019 13:34
Operator : AJ\SJ
Sample : K1389-06 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 08 22:44:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

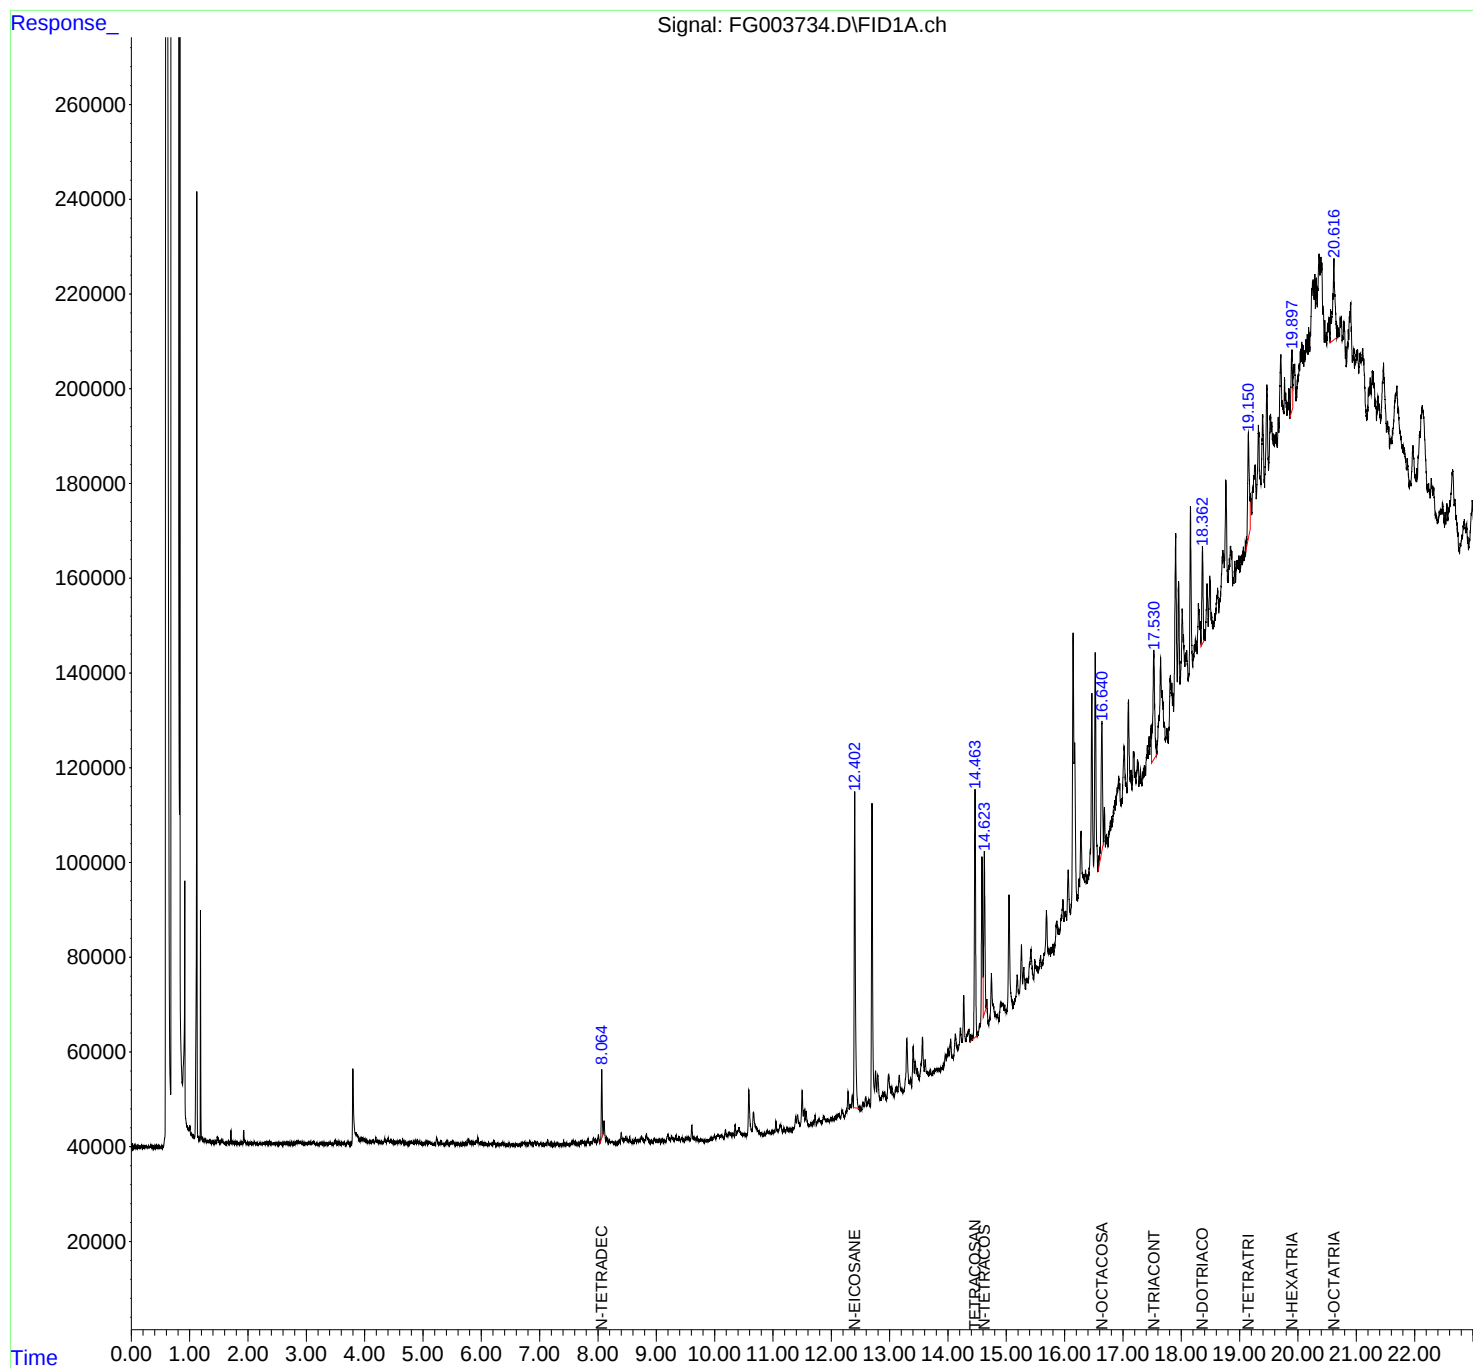

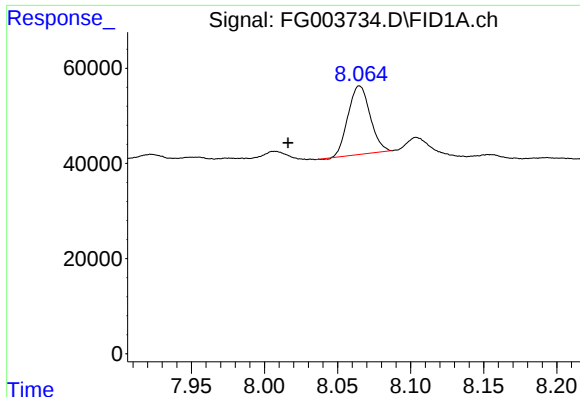


#4 N-TETRADECANE

R.T.: 8.065 min
Delta R.T.: 0.049 min
Response: 151003
Conc: 0.96 ug/ml

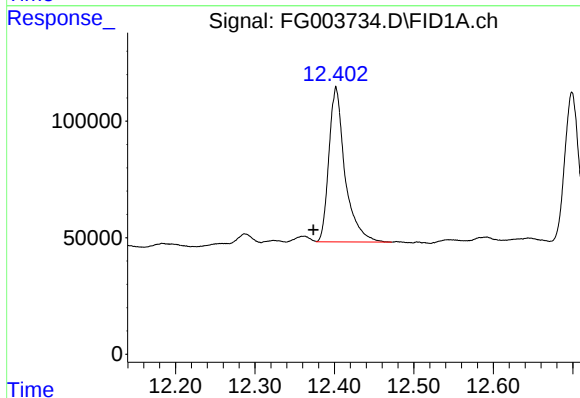


#7 N-EICOSANE

R.T.: 12.402 min
Delta R.T.: 0.029 min
Response: 933436
Conc: 5.96 ug/ml

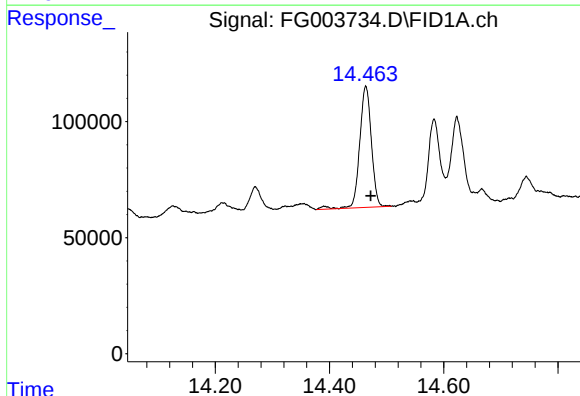


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.464 min
Delta R.T.: -0.009 min
Response: 743709
Conc: 5.50 ug/ml

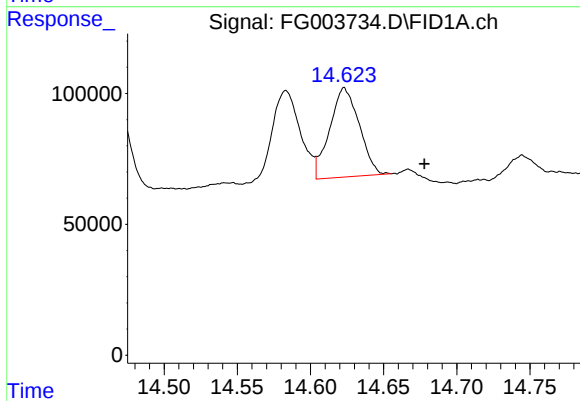


#10 N-TETRACOSANE

R.T.: 14.623 min
Delta R.T.: -0.055 min
Response: 478262
Conc: 3.17 ug/ml

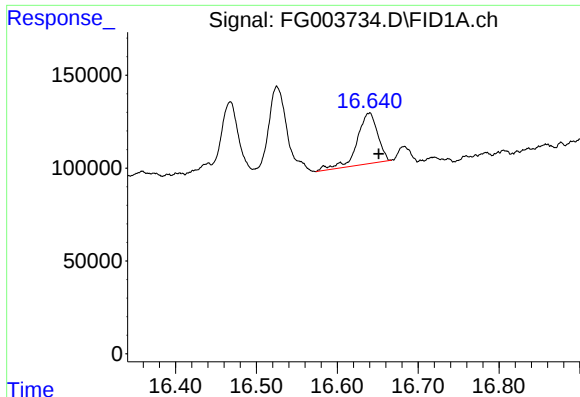


#12 N-OCTACOSANE

R.T.: 16.640 min
Delta R.T.: -0.012 min
Response: 481875
Conc: 3.34 ug/ml

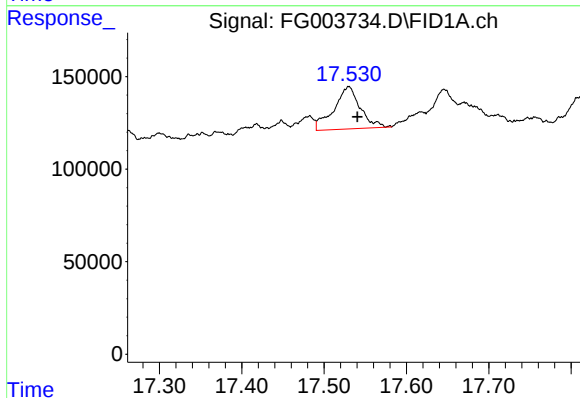


#13 N-TRIACONTANE

R.T.: 17.530 min
Delta R.T.: -0.010 min
Response: 506051
Conc: 3.58 ug/ml

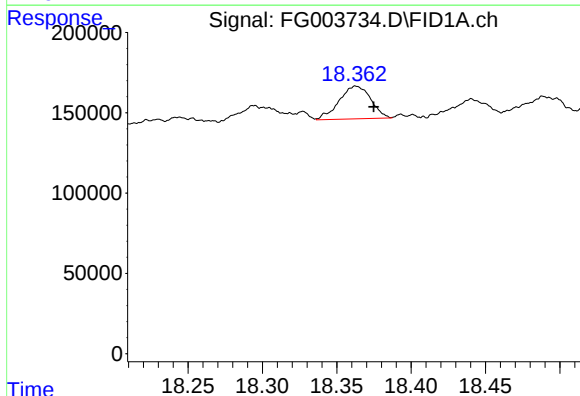


#14 N-DOTRIACONTANE

R.T.: 18.363 min
Delta R.T.: -0.012 min
Response: 301978
Conc: 2.31 ug/ml

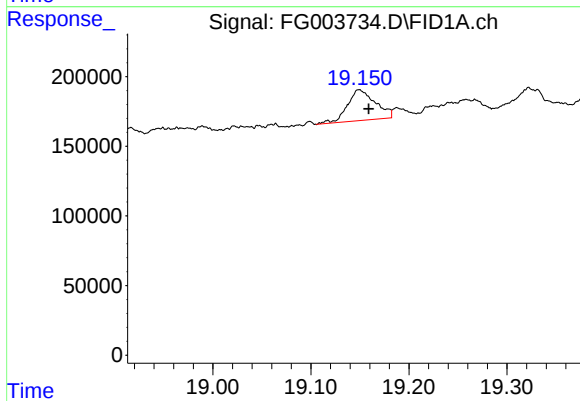


#15 N-TETRATRIACONTANE

R.T.: 19.149 min
Delta R.T.: -0.010 min
Response: 437657
Conc: 3.71 ug/ml

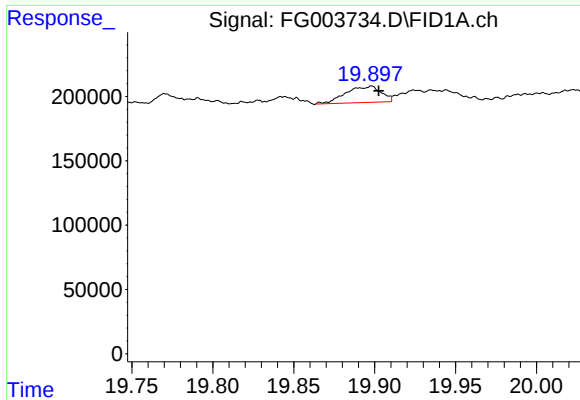

#16 N-HEXATRIACONTANE

R.T.: 19.898 min
Delta R.T.: -0.005 min
Response: 191680
Conc: 1.82 ug/ml

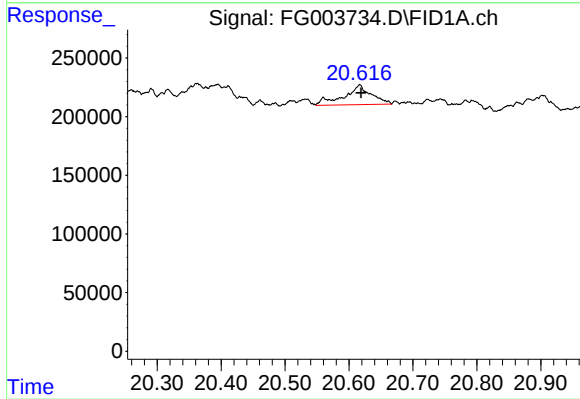

#17 N-OCTATRIACONTANE

R.T.: 20.616 min
Delta R.T.: -0.002 min
Response: 495891
Conc: 5.07 ug/ml