

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021022\
Data File : FG009365.D
Signal(s) : FID1A.ch
Acq On : 10 Feb 2022 14:07
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 11 03:21:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021022.M
Quant Title :
QLast Update : Fri Feb 11 03:18:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.731	4713002	19.103 ug/ml

Target Compounds


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021022\
Data File : FG009365.D
Signal(s) : FID1A.ch
Acq On : 10 Feb 2022 14:07
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 11 03:21:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021022.M
Quant Title :
QLast Update : Fri Feb 11 03:18:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

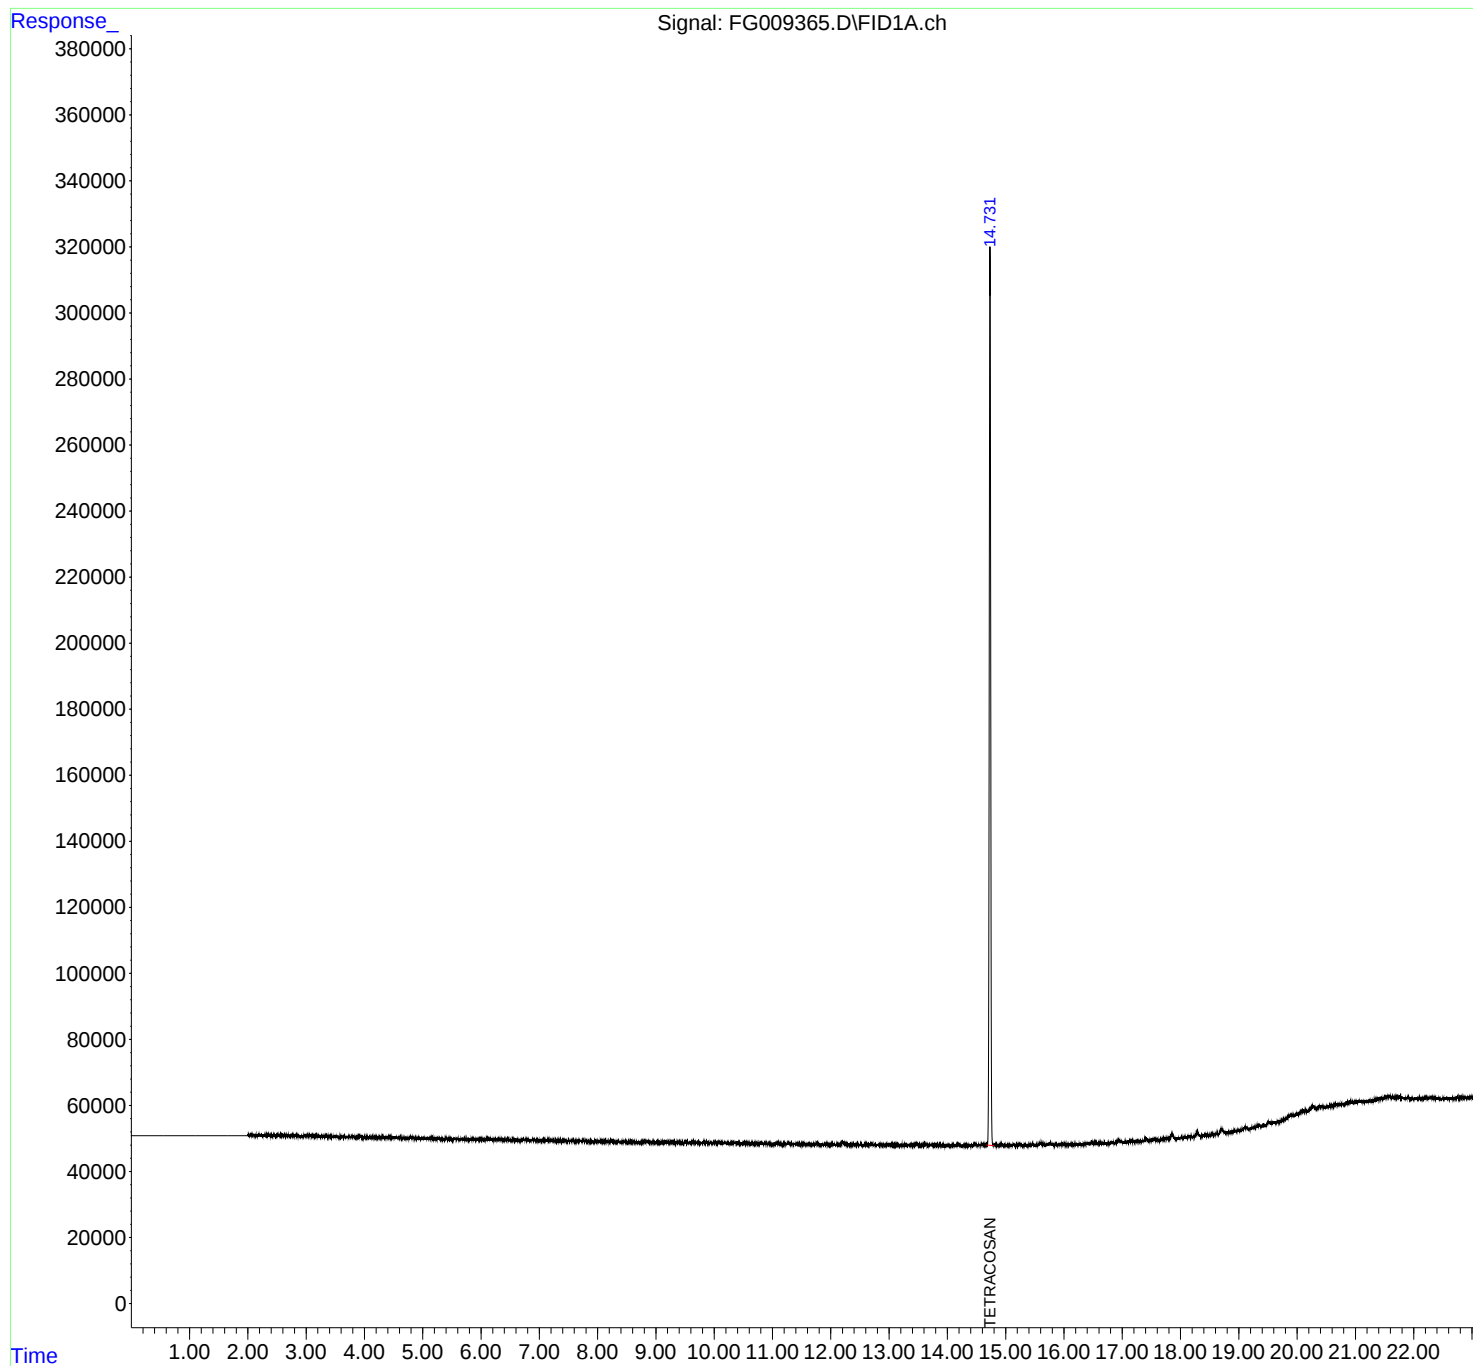

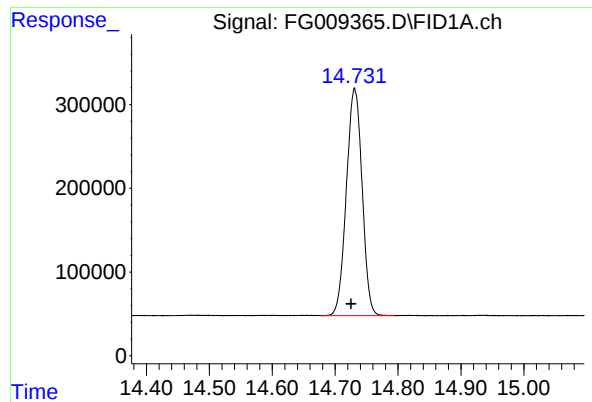

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.731 min
Delta R.T.: 0.005 min
Response: 4713002
Conc: 19.10 ug/ml