

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021120\
 Data File : FG006673.D
 Signal(s) : FID1A.ch
 Acq On : 11 Feb 2020 16:32
 Operator : DD\AJ
 Sample : L1439-02 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 12 00:26:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
 Quant Title :
 QLast Update : Tue Feb 11 13:28:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.612	341595	3.356 ug/ml
Target Compounds			
7) N-EICOSANE	12.576	120370	1.072 ug/ml
8) N-DOCOSANE	13.705	68037	0.593 ug/ml
10) N-TETRACOSANE	14.823	394645	3.396 ug/ml
12) N-OCTACOSANE	16.721	348159	2.957 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021120\
Data File : FG006673.D
Signal(s) : FID1A.ch
Acq On : 11 Feb 2020 16:32
Operator : DD\AJ
Sample : L1439-02 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 12 00:26:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

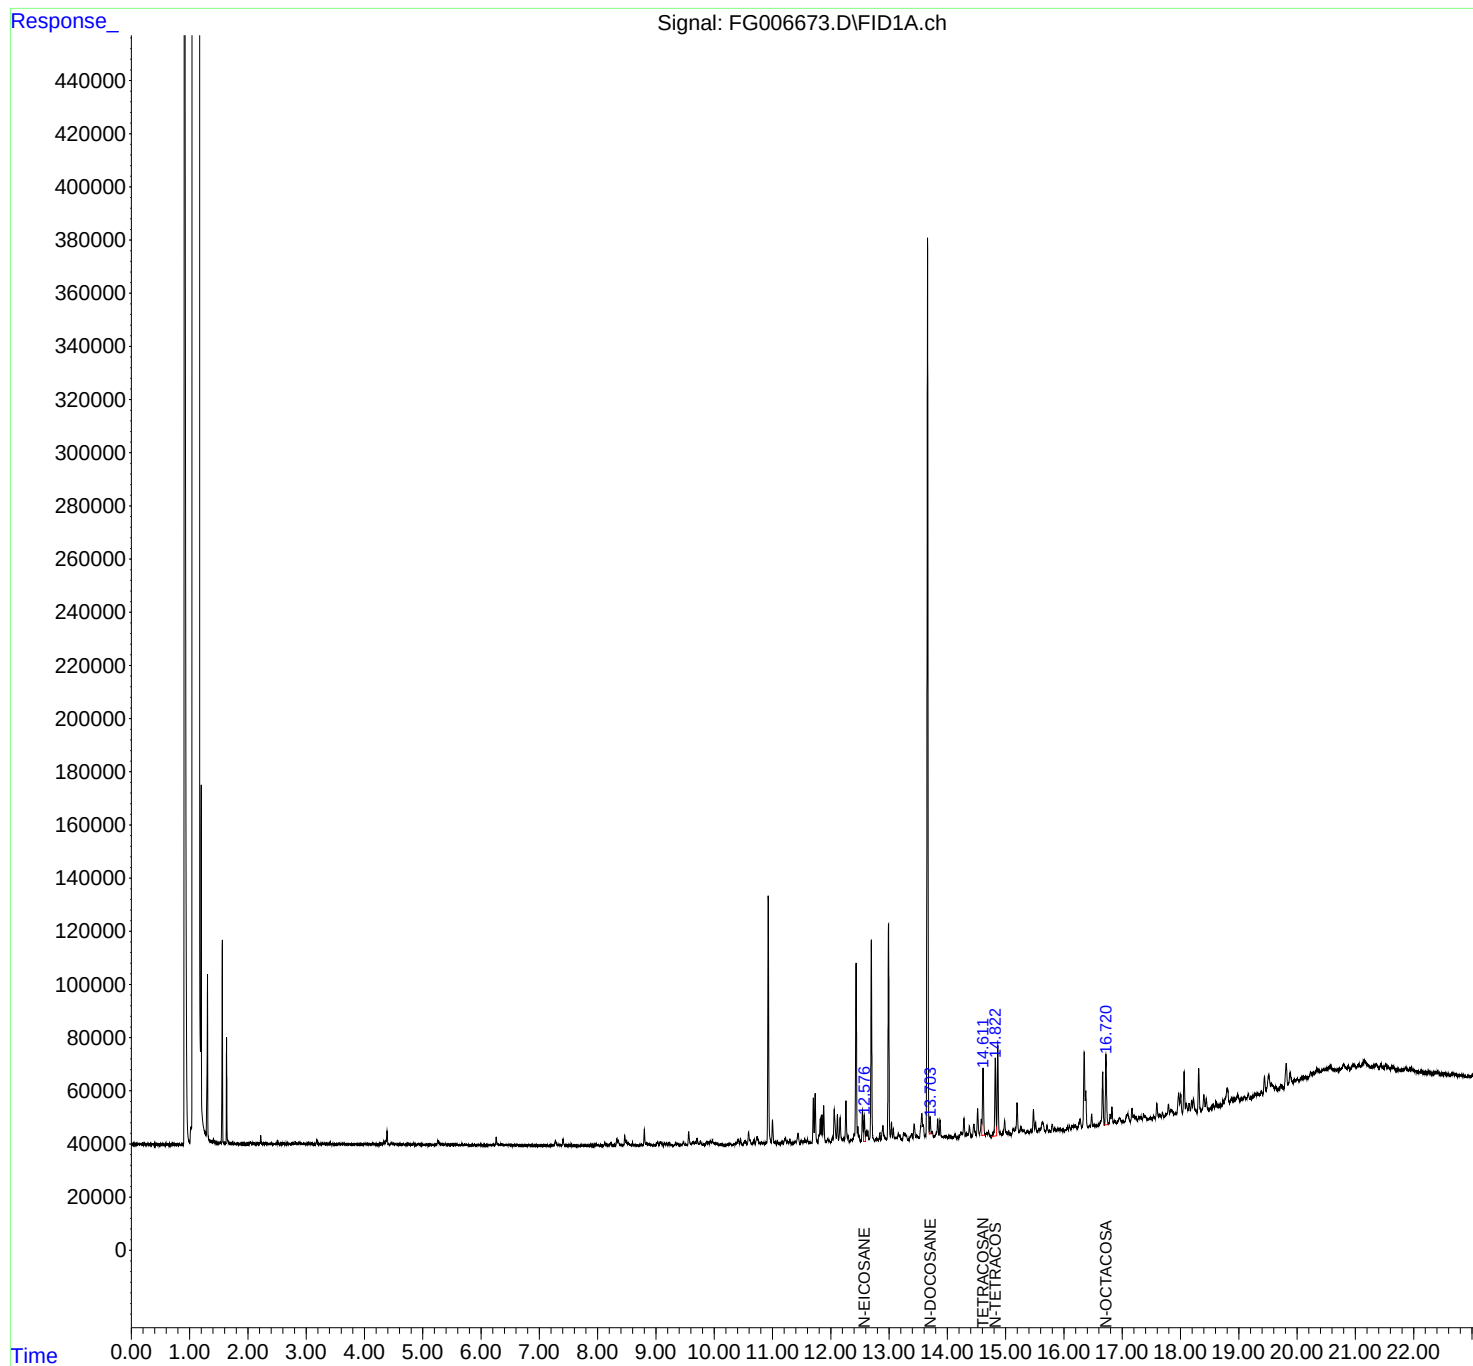


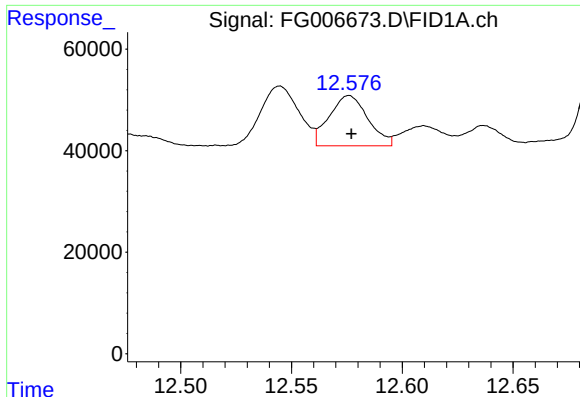

#7 N-EICOSANE


R.T.: 12.576 min
Delta R.T.: 0.000 min
Response: 120370
Conc: 1.07 ug/ml

Instrument :
FID_G
ClientSampleId :

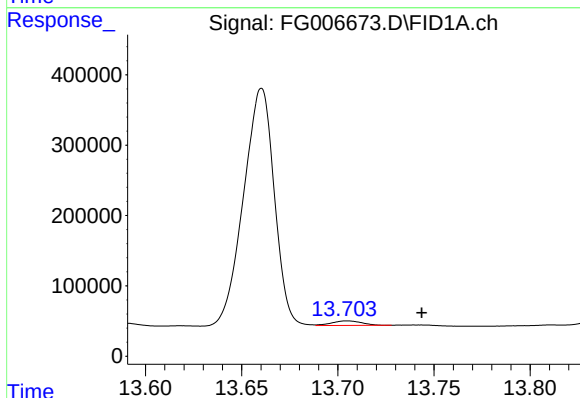


#8 N-DOCOSANE

R.T.: 13.705 min
Delta R.T.: -0.038 min
Response: 68037
Conc: 0.59 ug/ml

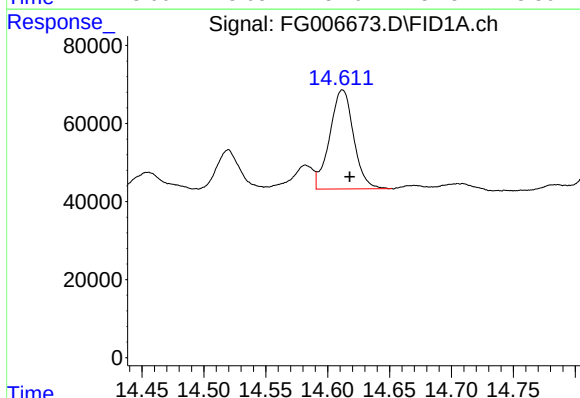


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.612 min
Delta R.T.: -0.006 min
Response: 341595
Conc: 3.36 ug/ml

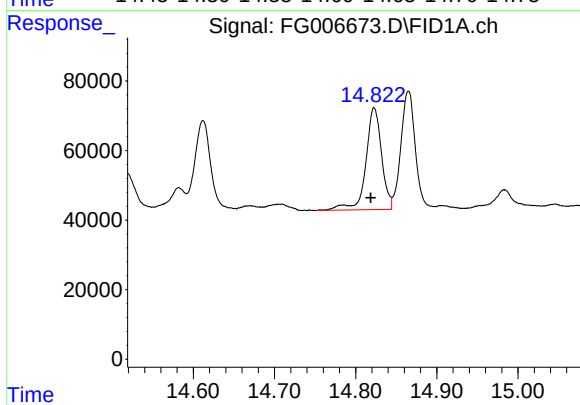

#10 N-TETRACOSANE

R.T.: 14.823 min
Delta R.T.: 0.005 min
Response: 394645
Conc: 3.40 ug/ml

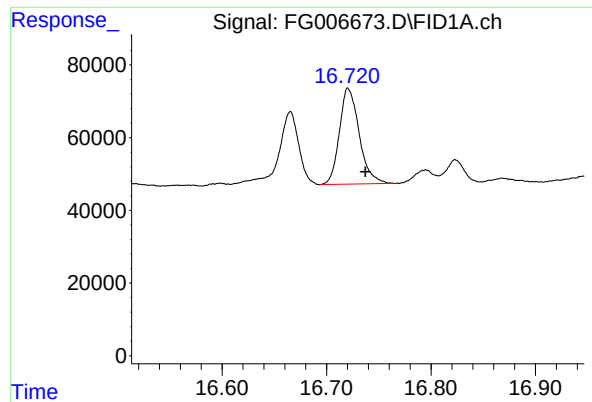

#12 N-OCTACOSANE

R.T.: 16.721 min
Delta R.T.: -0.016 min
Response: 348159
Conc: 2.96 ug/ml

Instrument :
FID_G
ClientSampleId :