

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID\_G\Data\FG021219\  
Data File : FG003756.D  
Signal(s) : FID1A.ch  
Acq On : 12 Feb 2019 10:07  
Operator : AJ\SJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 12 12:12:23 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG020519.M  
Quant Title :  
QLast Update : Wed Feb 06 08:50:01 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.213  | 2685315  | 17.008 ug/ml |
| 12) N-OCTACOSANE            | 16.636 | 2507225  | 17.402 ug/ml |
| 14) N-DOTRIACONTANE         | 18.355 | 197253   | 1.506 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID\_G\Data\FG021219\  
Data File : FG003756.D  
Signal(s) : FID1A.ch  
Acq On : 12 Feb 2019 10:07  
Operator : AJ\SJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 12 12:12:23 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG020519.M  
Quant Title :  
QLast Update : Wed Feb 06 08:50:01 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

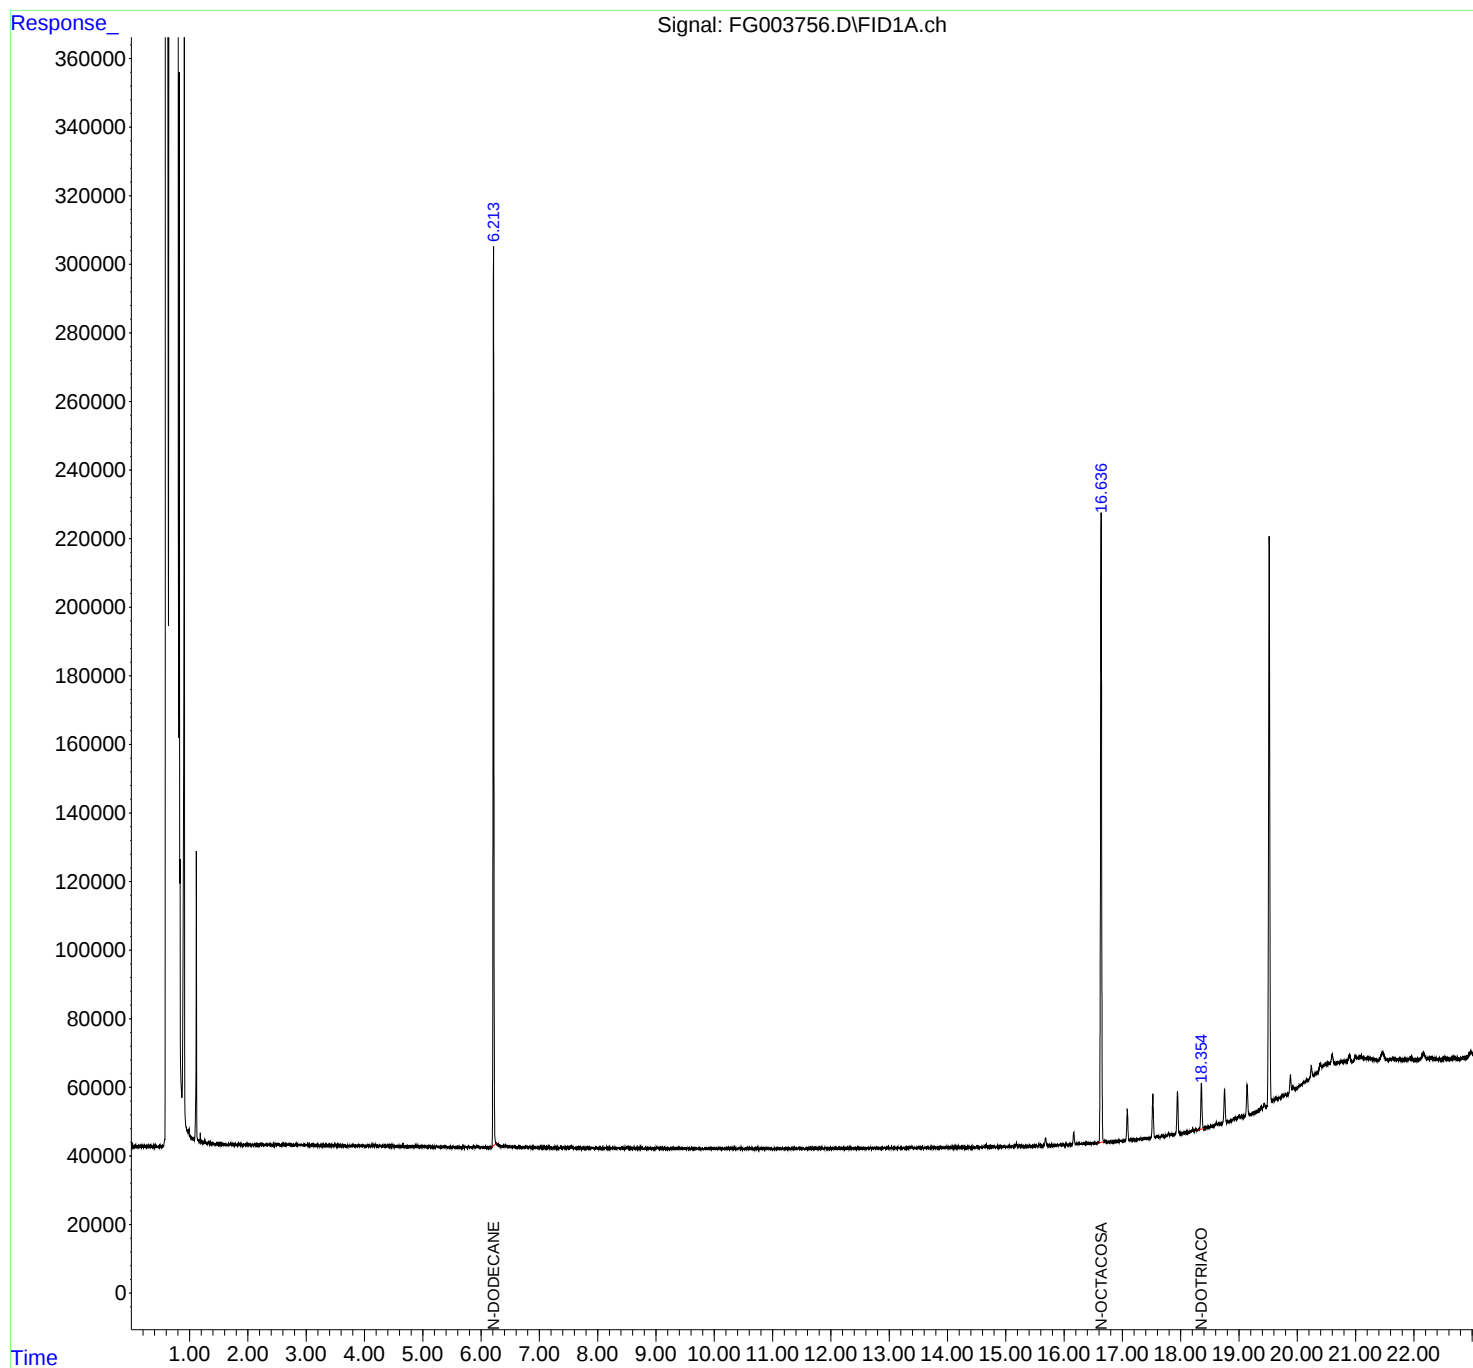


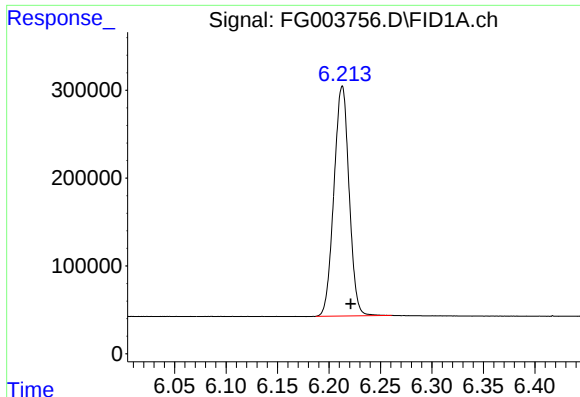

#3 N-DODECANE


R.T.: 6.213 min  
Delta R.T.: -0.008 min  
Response: 2685315  
Conc: 17.01 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

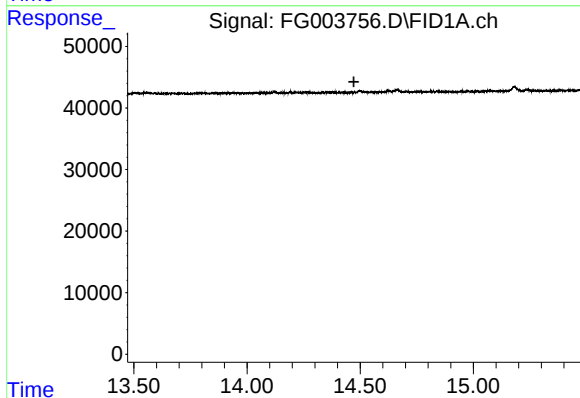


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.472 min  
Response: 0  
Conc: N.D.

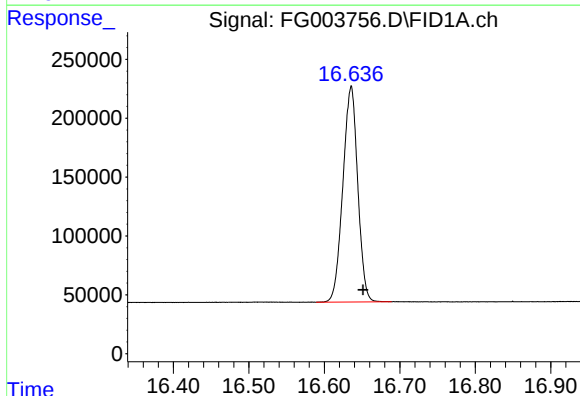

#12 N-OCTACOSANE

R.T.: 16.636 min  
Delta R.T.: -0.016 min  
Response: 2507225  
Conc: 17.40 ug/ml

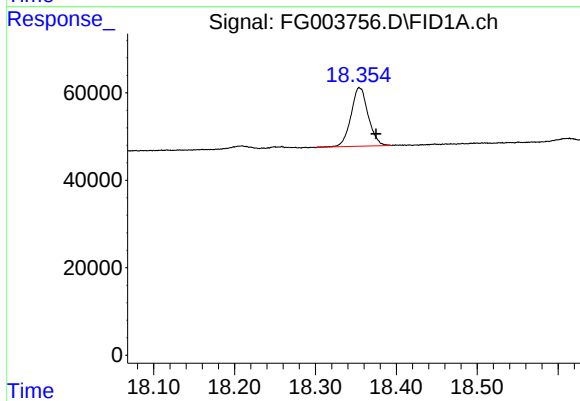

#14 N-DOTRIACONTANE

R.T.: 18.355 min  
Delta R.T.: -0.020 min  
Response: 197253  
Conc: 1.51 ug/ml