

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
 Data File : FG003758.D
 Signal(s) : FID1A.ch
 Acq On : 12 Feb 2019 11:11
 Operator : AJ\SJ
 Sample : K1423-02 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 12 12:12:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	654833	4.841 ug/ml
Target Compounds			
4) N-TETRADECANE	8.006	319168	2.022 ug/ml
5) N-HEXADECANE	9.606	736035	4.672 ug/ml
6) N-OCTADECANE	11.049	629903	4.001 ug/ml
7) N-EICOSANE	12.360	448089	2.861 ug/ml
8) N-DOCOSANE	13.558	223188	1.443 ug/ml
10) N-TETRACOSANE	14.621f	157561	1.046 ug/ml
12) N-OCTACOSANE	16.633	338885	2.352 ug/ml
13) N-TRIACONTANE	17.522	490708	3.467 ug/ml
14) N-DOTRIACONTANE	18.354	464733	3.549 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
Data File : FG003758.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2019 11:11
Operator : AJ\SJ
Sample : K1423-02 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 12 12:12:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

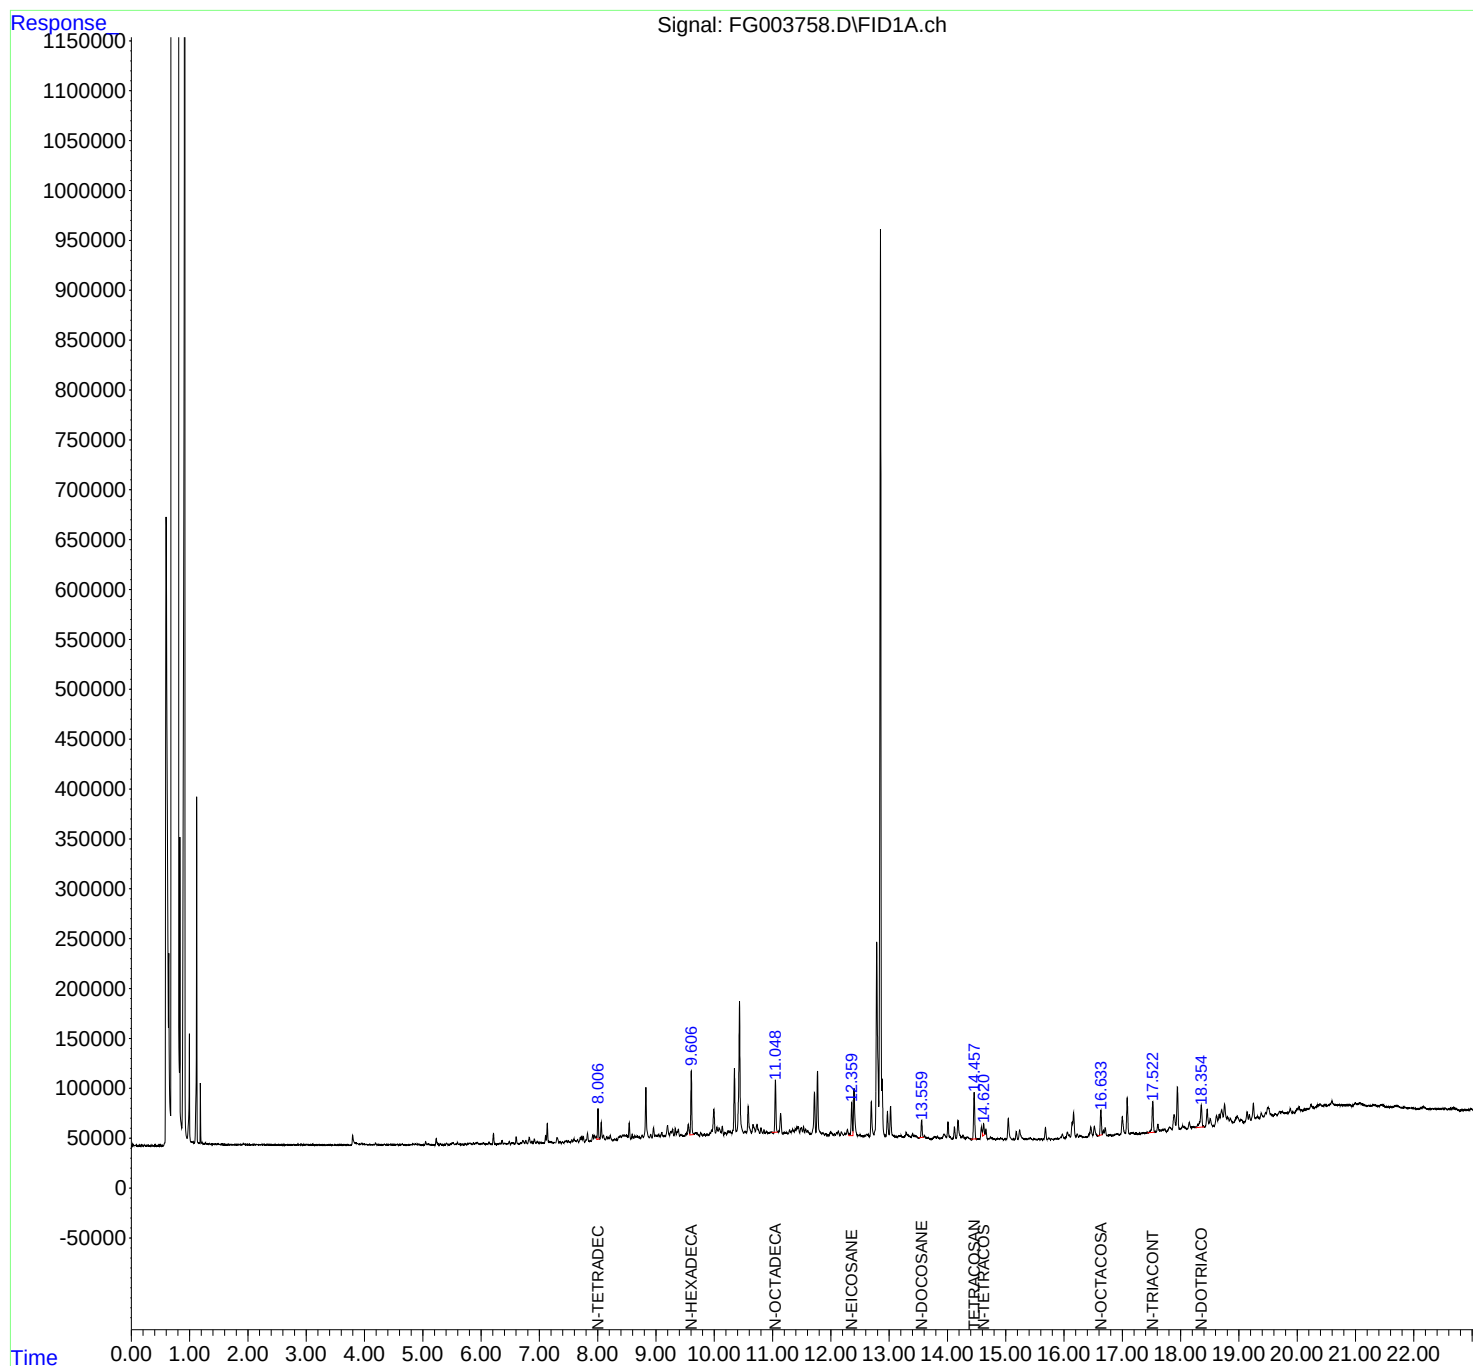


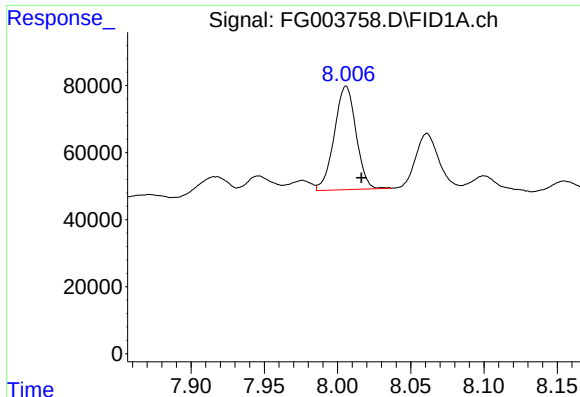

#4 N-TETRADECANE


R.T.: 8.006 min
Delta R.T.: -0.010 min
Response: 319168
Conc: 2.02 ug/ml

Instrument :
FID_G
ClientSampleId :

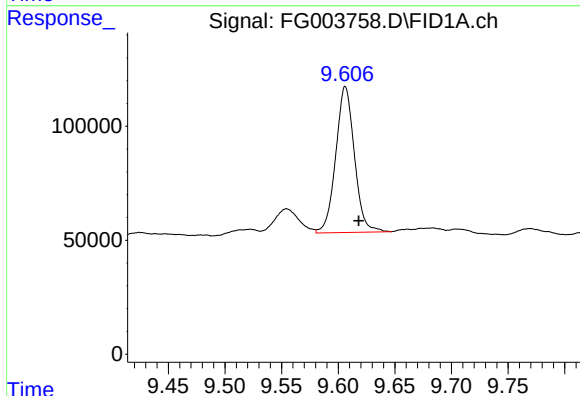


#5 N-HEXADECANE

R.T.: 9.606 min
Delta R.T.: -0.012 min
Response: 736035
Conc: 4.67 ug/ml

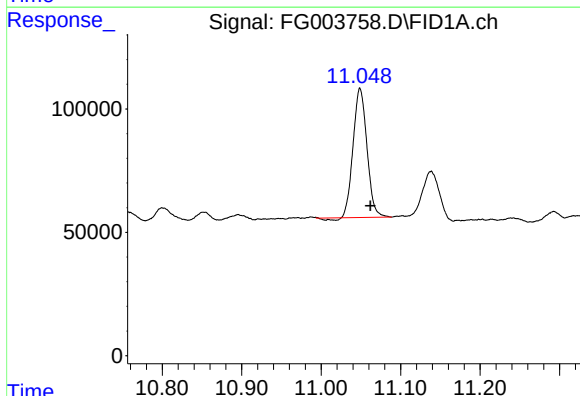


#6 N-OCTADECANE

R.T.: 11.049 min
Delta R.T.: -0.013 min
Response: 629903
Conc: 4.00 ug/ml

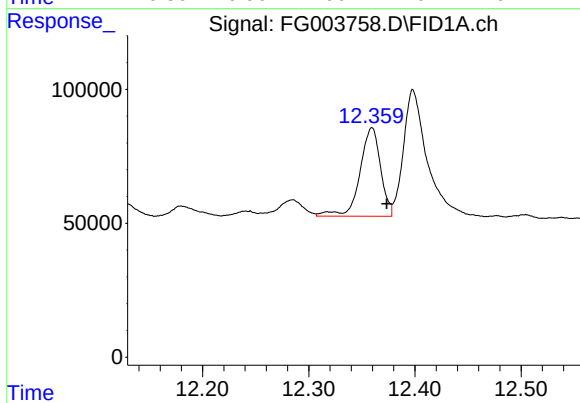

#7 N-EICOSANE


R.T.: 12.360 min
Delta R.T.: -0.014 min
Response: 448089
Conc: 2.86 ug/ml

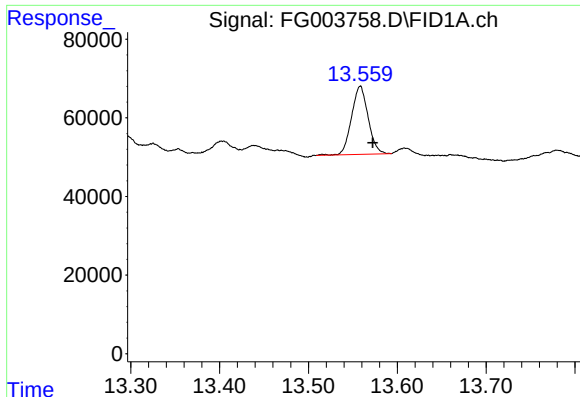

#8 N-DOCOSANE


R.T.: 13.558 min
Delta R.T.: -0.014 min
Response: 223188
Conc: 1.44 ug/ml

Instrument :
FID_G
ClientSampleId :

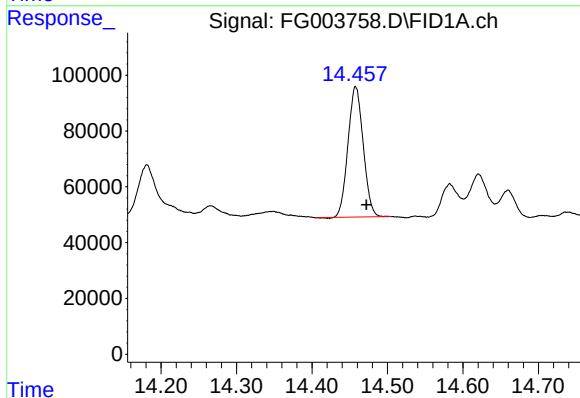


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.014 min
Response: 654833
Conc: 4.84 ug/ml

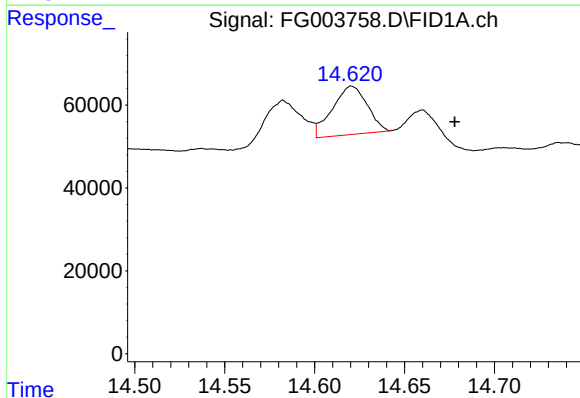


#10 N-TETRACOSANE

R.T.: 14.621 min
Delta R.T.: -0.057 min
Response: 157561
Conc: 1.05 ug/ml

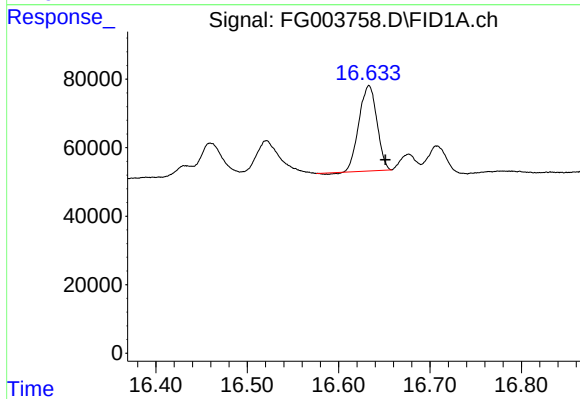

#12 N-OCTACOSANE


R.T.: 16.633 min
Delta R.T.: -0.018 min
Response: 338885
Conc: 2.35 ug/ml

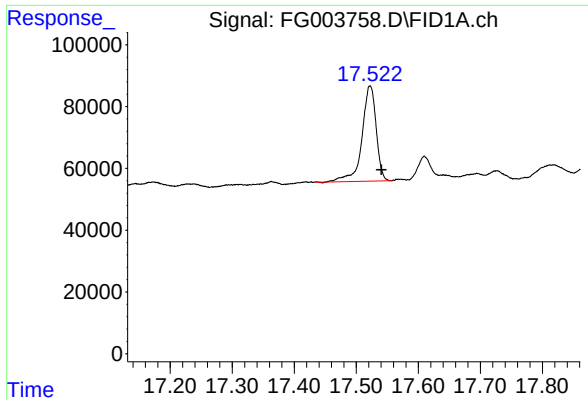

#13 N-TRIACONTANE

R.T.: 17.522 min
Delta R.T.: -0.018 min
Response: 490708
Conc: 3.47 ug/ml

Instrument :
FID_G
ClientSampleId :

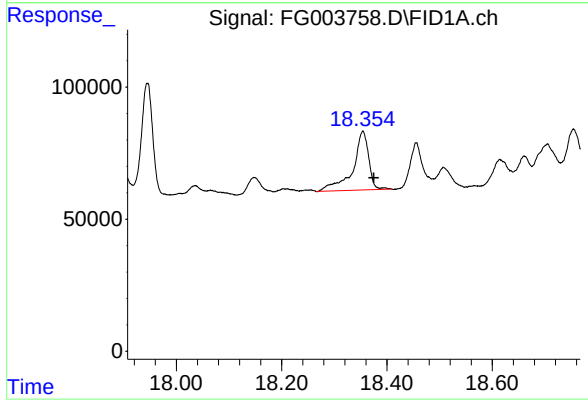

#14 N-DOTRIACONTANE

R.T.: 18.354 min
Delta R.T.: -0.021 min
Response: 464733
Conc: 3.55 ug/ml