

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
Data File : FG003765.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2019 16:03
Operator : AJ\SJ
Sample : K1437-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 00:17:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.462	1582965	11.703 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.362	174444	1.332 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
Data File : FG003765.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2019 16:03
Operator : AJ\SJ
Sample : K1437-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 00:17:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

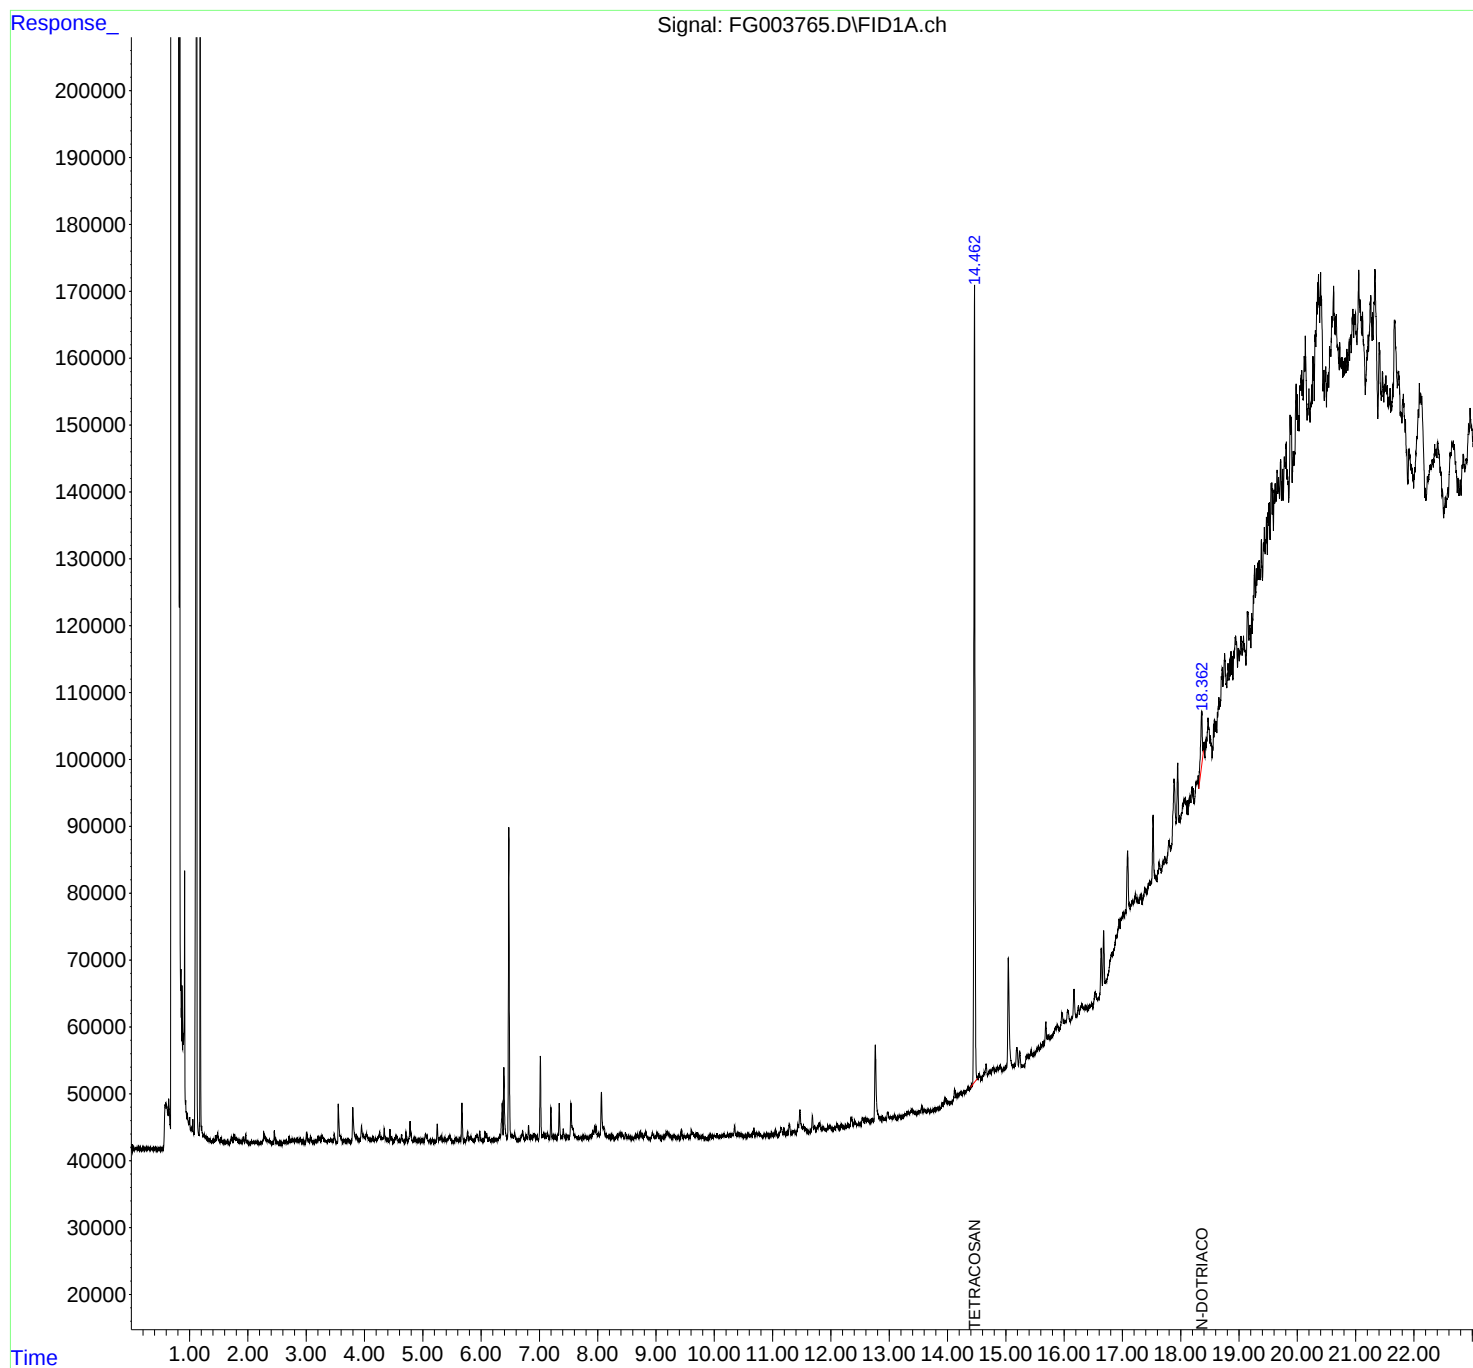


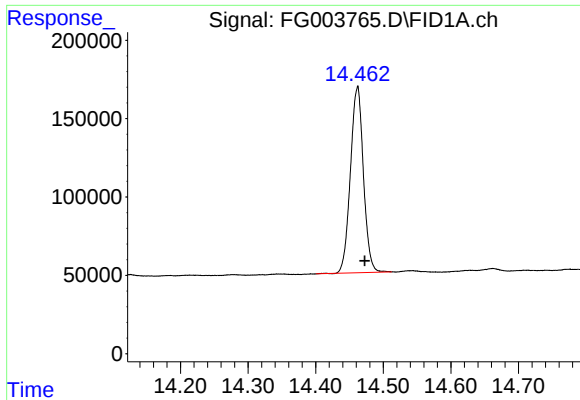

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.462 min
Delta R.T.: -0.010 min
Response: 1582965
Conc: 11.70 ug/ml

Instrument :
FID_G
ClientSampleId :

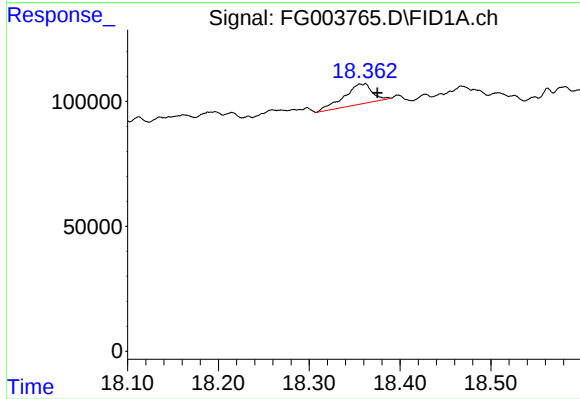

#14 N-DOTRIACONTANE

R.T.: 18.362 min
Delta R.T.: -0.013 min
Response: 174444
Conc: 1.33 ug/ml