

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
 Data File : FG003766.D
 Signal(s) : FID1A.ch
 Acq On : 12 Feb 2019 16:33
 Operator : AJ\SJ
 Sample : K1459-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 13 00:17:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.461	1505777	11.133 ug/ml
Target Compounds			
4) N-TETRADECANE	8.062	282097	1.787 ug/ml
7) N-EICOSANE	12.399	1156688	7.385 ug/ml
10) N-TETRACOSANE	14.621f	802548	5.326 ug/ml
12) N-OCTACOSANE	16.633	468639	3.253 ug/ml
13) N-TRIACONTANE	17.525	546850	3.864 ug/ml
14) N-DOTRIACONTANE	18.357	260926	1.993 ug/ml
15) N-TETRATRIACONTANE	19.150	265381	2.250 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
Data File : FG003766.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2019 16:33
Operator : AJ\SJ
Sample : K1459-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 00:17:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

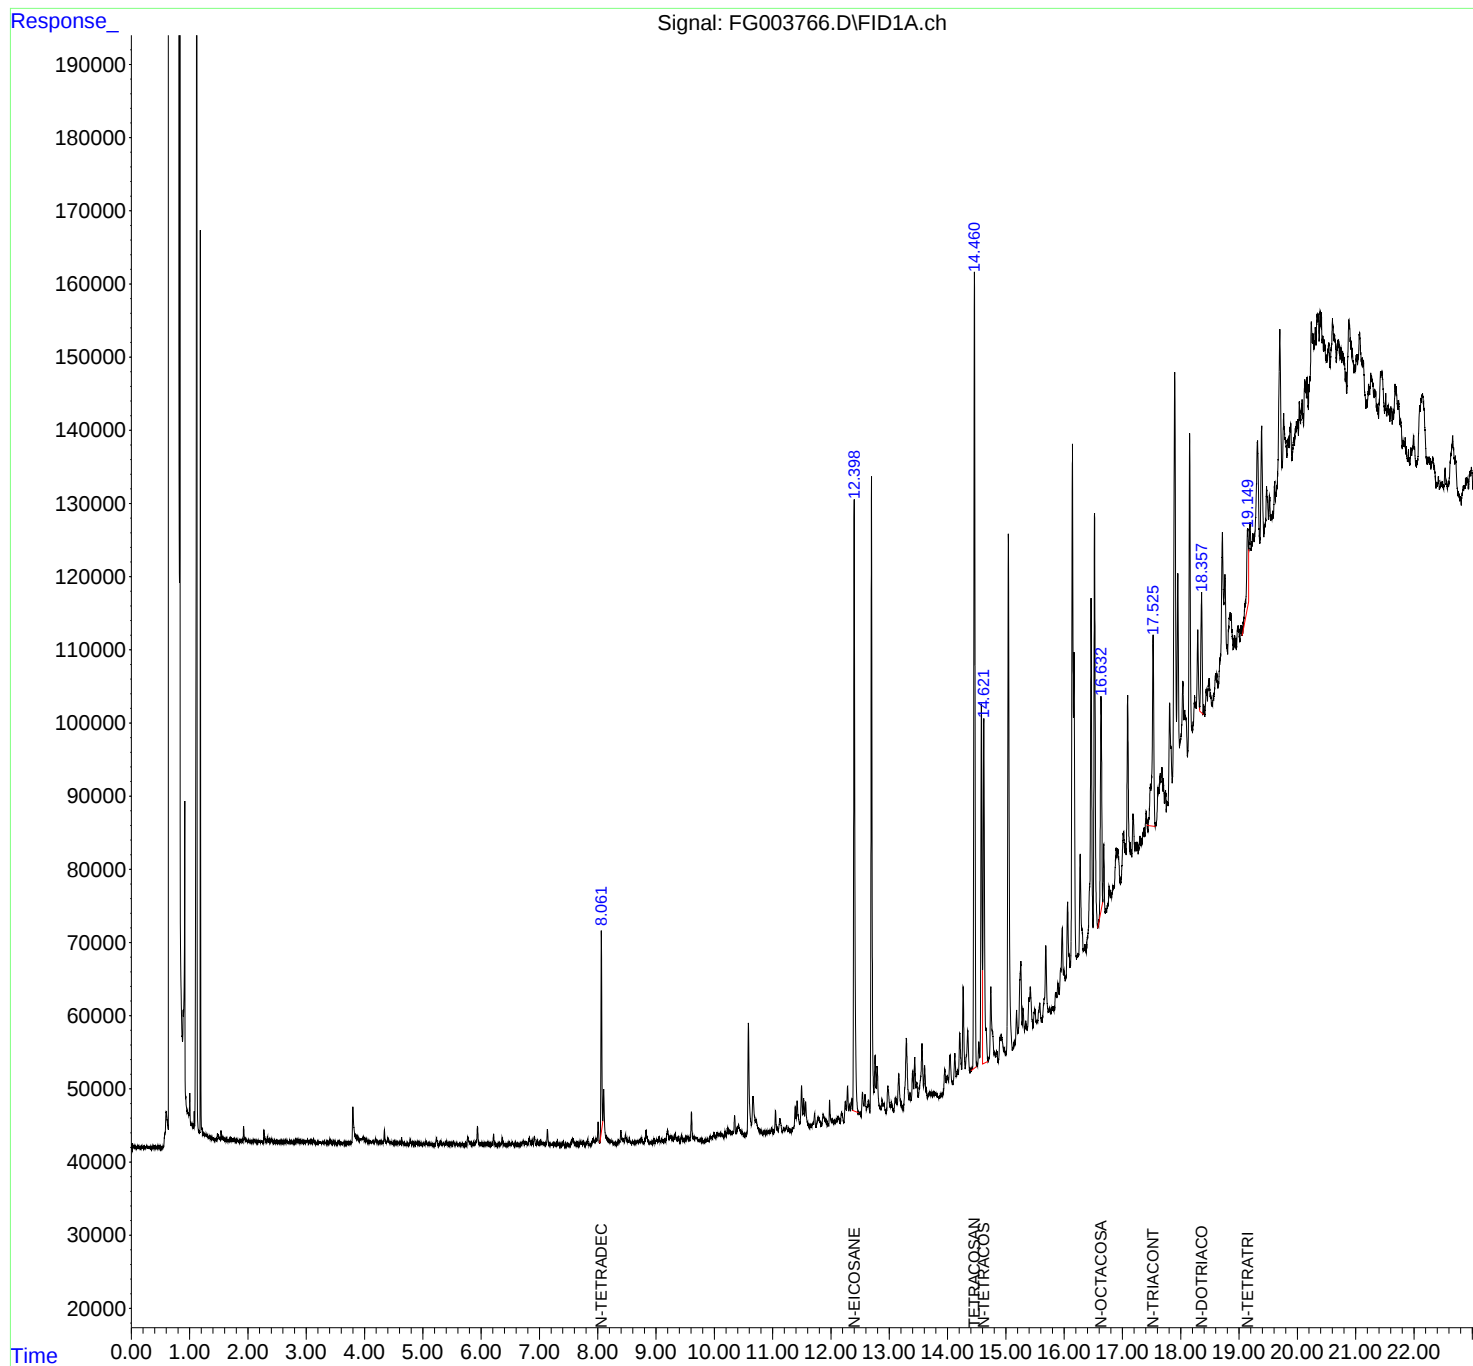


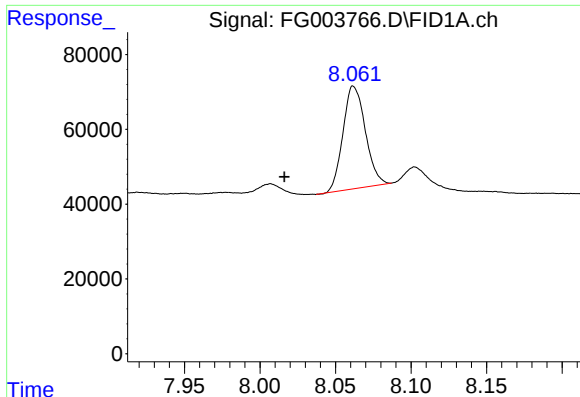

#4 N-TETRADECANE


R.T.: 8.062 min
Delta R.T.: 0.046 min
Response: 282097
Conc: 1.79 ug/ml

Instrument :
FID_G
ClientSampleId :

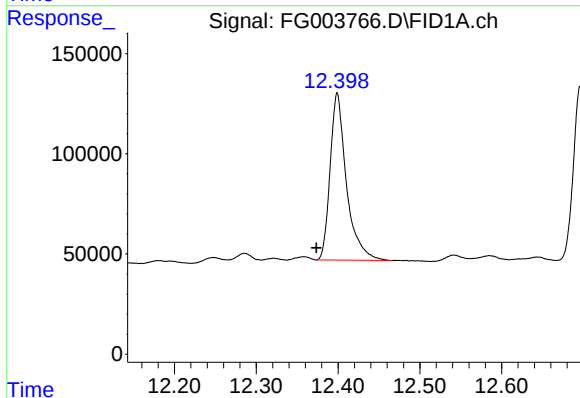


#7 N-EICOSANE

R.T.: 12.399 min
Delta R.T.: 0.026 min
Response: 1156688
Conc: 7.39 ug/ml

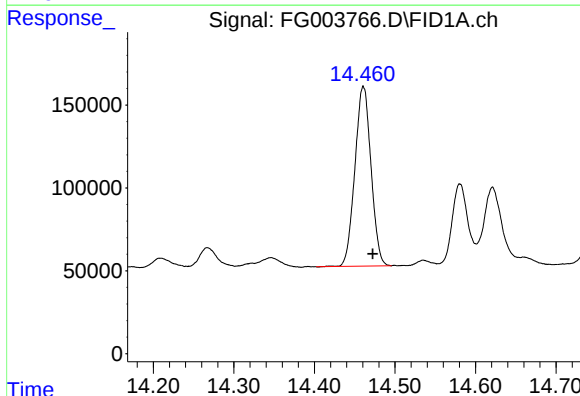


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.461 min
Delta R.T.: -0.011 min
Response: 1505777
Conc: 11.13 ug/ml

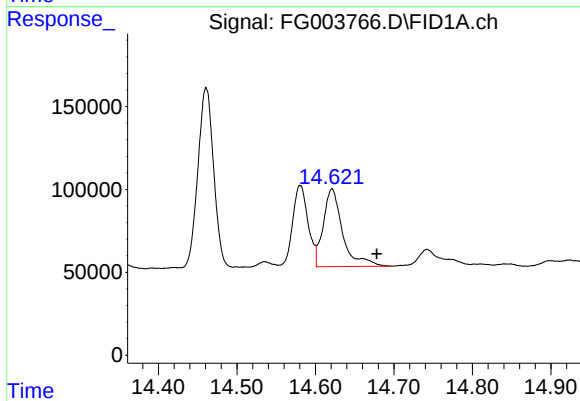

#10 N-TETRACOSANE


R.T.: 14.621 min
Delta R.T.: -0.057 min
Response: 802548
Conc: 5.33 ug/ml

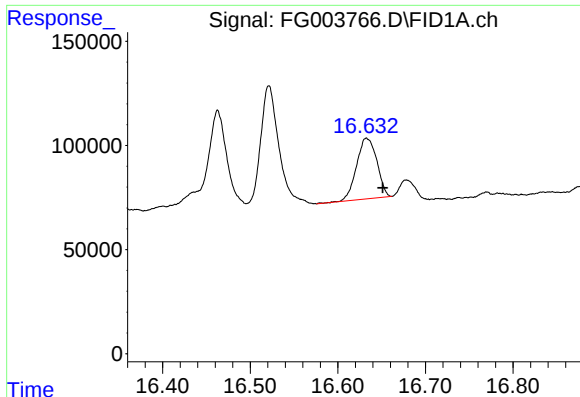

#12 N-OCTACOSANE


R.T.: 16.633 min
Delta R.T.: -0.019 min
Response: 468639
Conc: 3.25 ug/ml

Instrument :
FID_G
ClientSampleId :

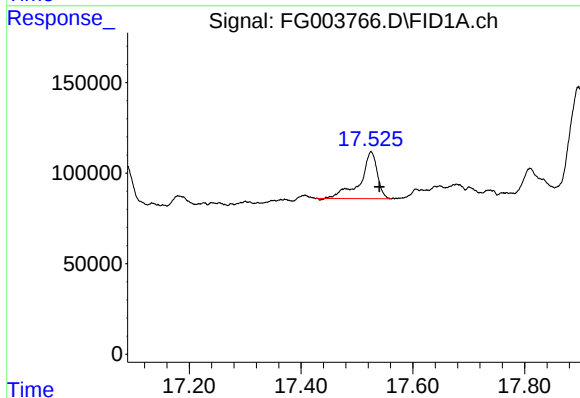


#13 N-TRIACONTANE

R.T.: 17.525 min
Delta R.T.: -0.015 min
Response: 546850
Conc: 3.86 ug/ml

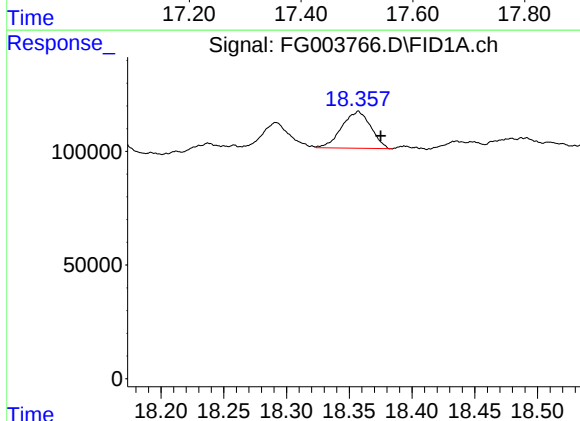

#14 N-DOTRIACONTANE

R.T.: 18.357 min
Delta R.T.: -0.018 min
Response: 260926
Conc: 1.99 ug/ml

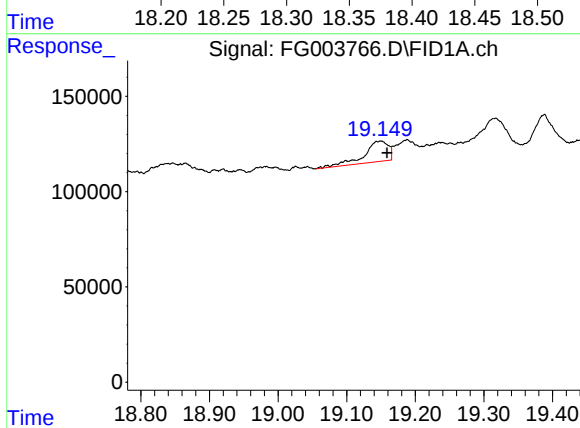

#15 N-TETRATRIACONTANE

R.T.: 19.150 min
Delta R.T.: -0.009 min
Response: 265381
Conc: 2.25 ug/ml