

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
Data File : FG003776.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2019 21:37
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 00:19:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.460	2129928	15.747 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.358	232641	1.777 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021219\
Data File : FG003776.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2019 21:37
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 00:19:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

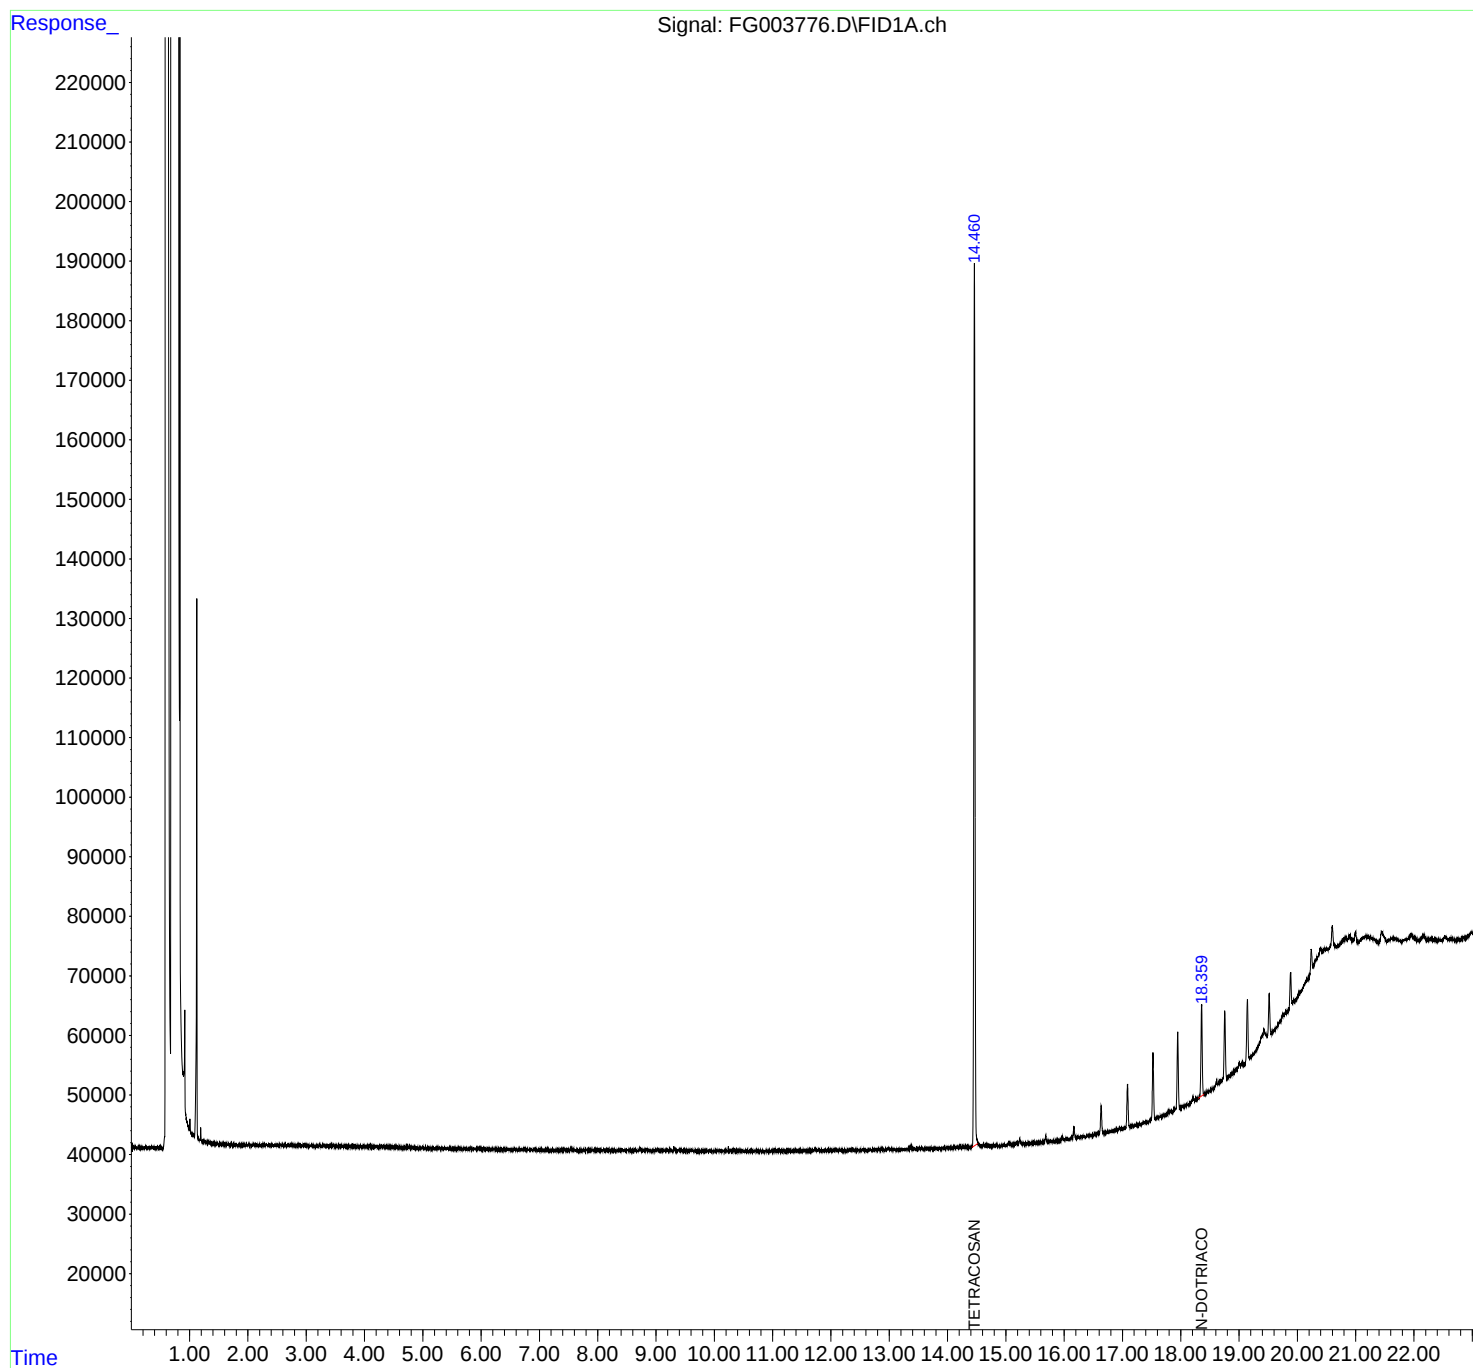


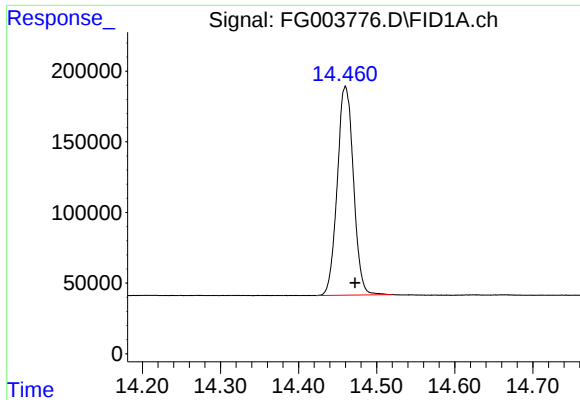

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.460 min
Delta R.T.: -0.012 min
Response: 2129928
Conc: 15.75 ug/ml

Instrument :
FID_G
ClientSampleId :

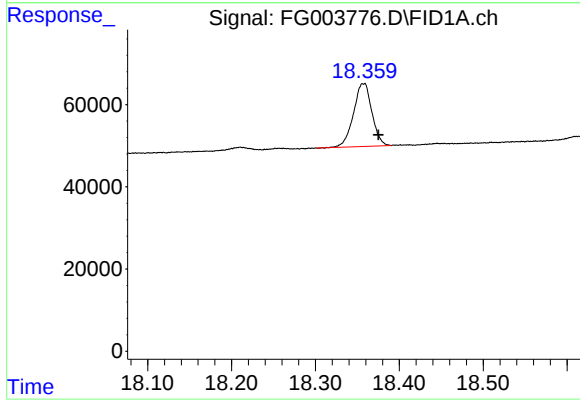

#14 N-DOTRIACONTANE

R.T.: 18.358 min
Delta R.T.: -0.017 min
Response: 232641
Conc: 1.78 ug/ml