

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
 Data File : FG006686.D
 Signal(s) : FID1A.ch
 Acq On : 12 Feb 2020 13:31
 Operator : DD\AJ
 Sample : L1491-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 13 02:25:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
 Quant Title :
 QLast Update : Tue Feb 11 13:28:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	1218665	11.973 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.730	97869	0.831 ug/ml
13) N-TRIACONTANE	17.594	132097	1.101 ug/ml
14) N-DOTRIACONTANE	18.402	91955	0.827 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
Data File : FG006686.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2020 13:31
Operator : DD\AJ
Sample : L1491-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 02:25:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

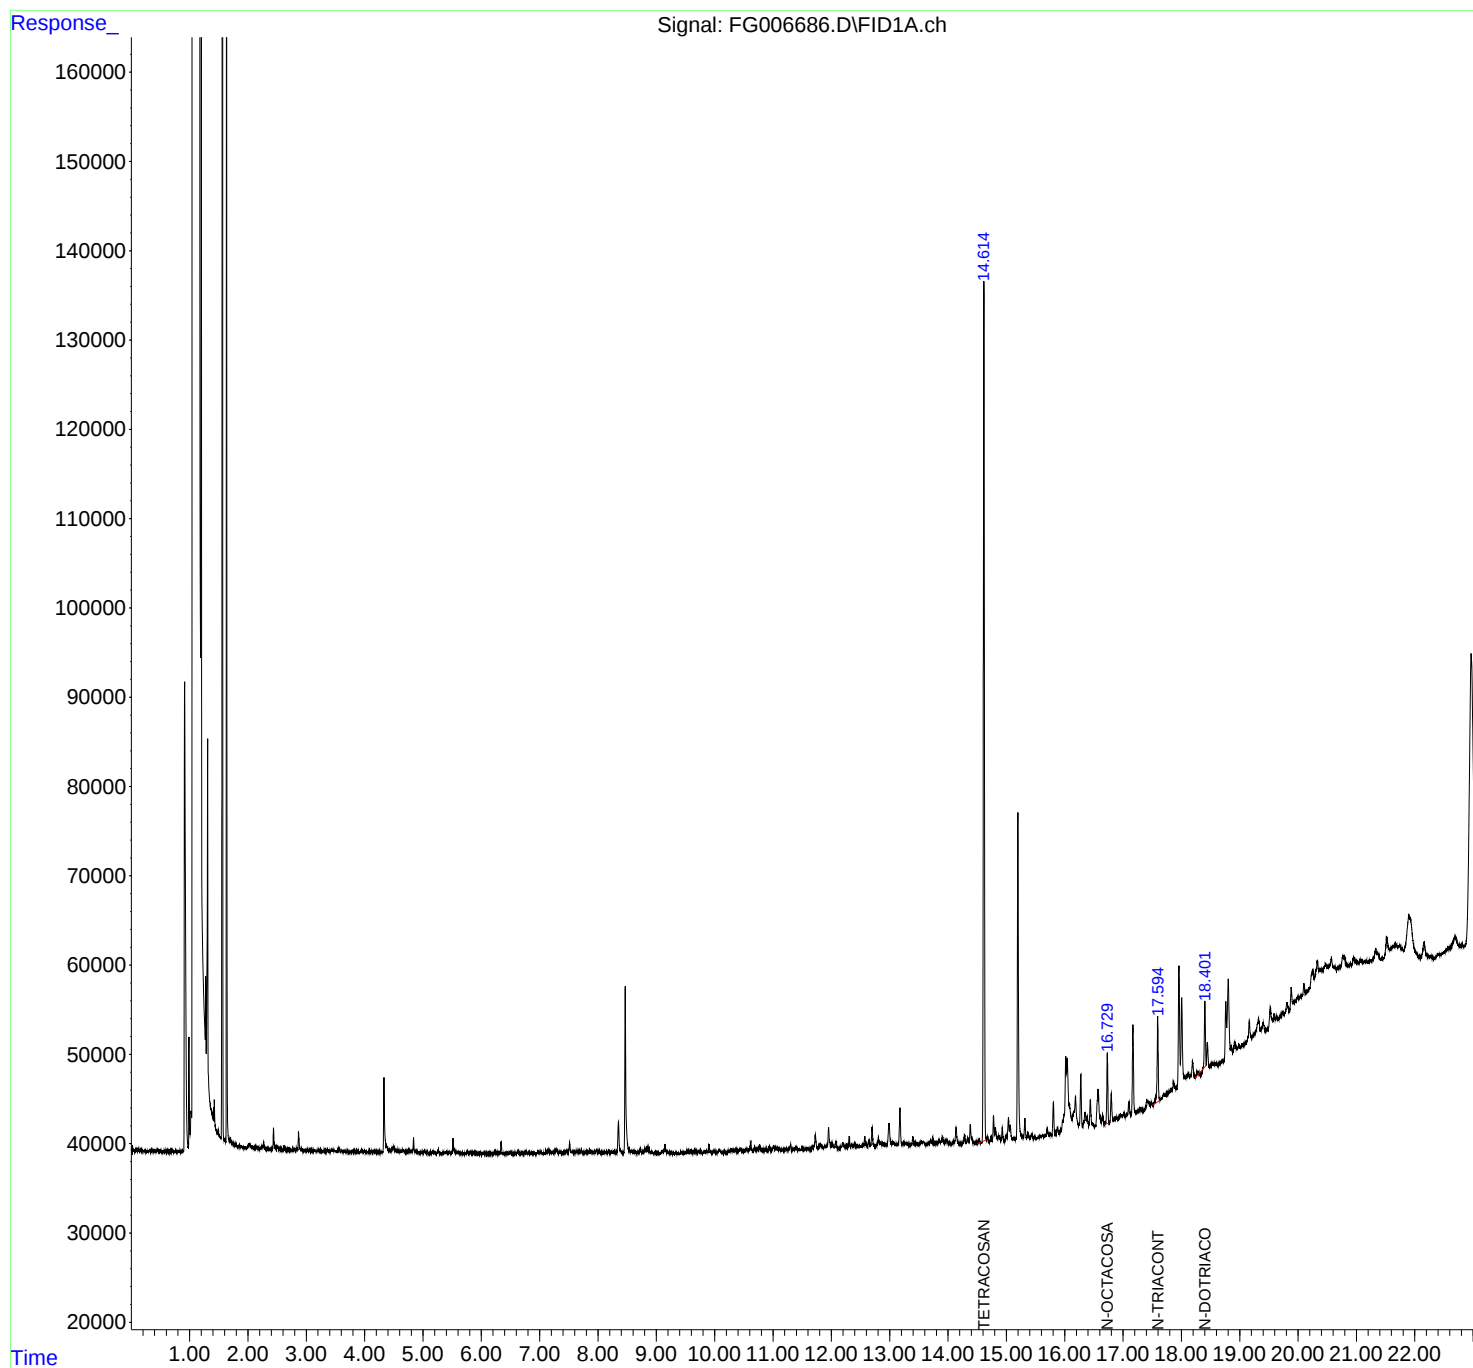


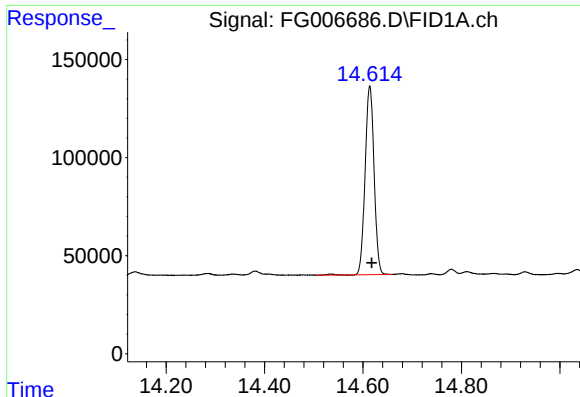

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.614 min
Delta R.T.: -0.004 min
Response: 1218665
Conc: 11.97 ug/ml

Instrument :
FID_G
ClientSampleId :

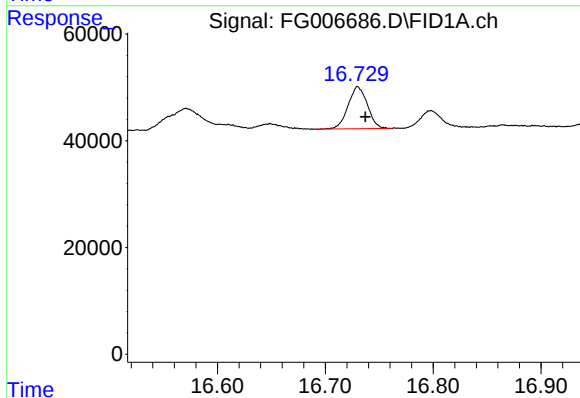


#12 N-OCTACOSANE

R.T.: 16.730 min
Delta R.T.: -0.007 min
Response: 97869
Conc: 0.83 ug/ml

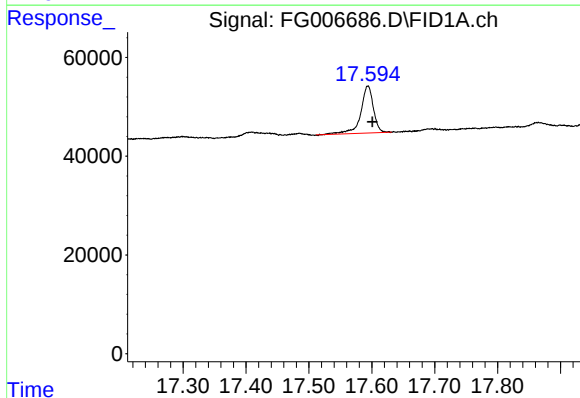

#13 N-TRIACONTANE

R.T.: 17.594 min
Delta R.T.: -0.007 min
Response: 132097
Conc: 1.10 ug/ml

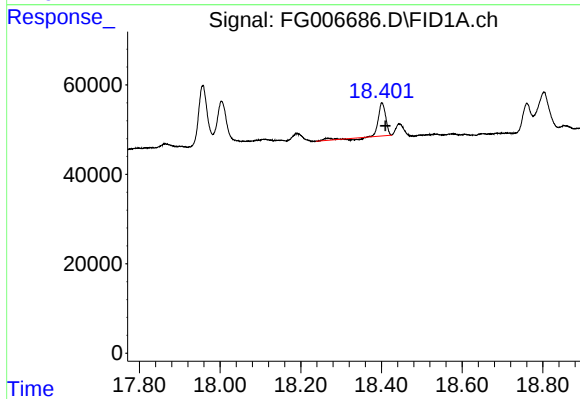

#14 N-DOTRIACONTANE

R.T.: 18.402 min
Delta R.T.: -0.009 min
Response: 91955
Conc: 0.83 ug/ml