

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
 Data File : FG006689.D
 Signal(s) : FID1A.ch
 Acq On : 12 Feb 2020 15:01
 Operator : DD\AJ
 Sample : L1491-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 13 02:28:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
 Quant Title :
 QLast Update : Tue Feb 11 13:28:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	1624908	15.965 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.805	72650	0.625 ug/ml
12) N-OCTACOSANE	16.729	149211	1.267 ug/ml
13) N-TRIACONTANE	17.592	181188	1.510 ug/ml
14) N-DOTRIACONTANE	18.400	74539	0.671 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
Data File : FG006689.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2020 15:01
Operator : DD\AJ
Sample : L1491-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 02:28:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

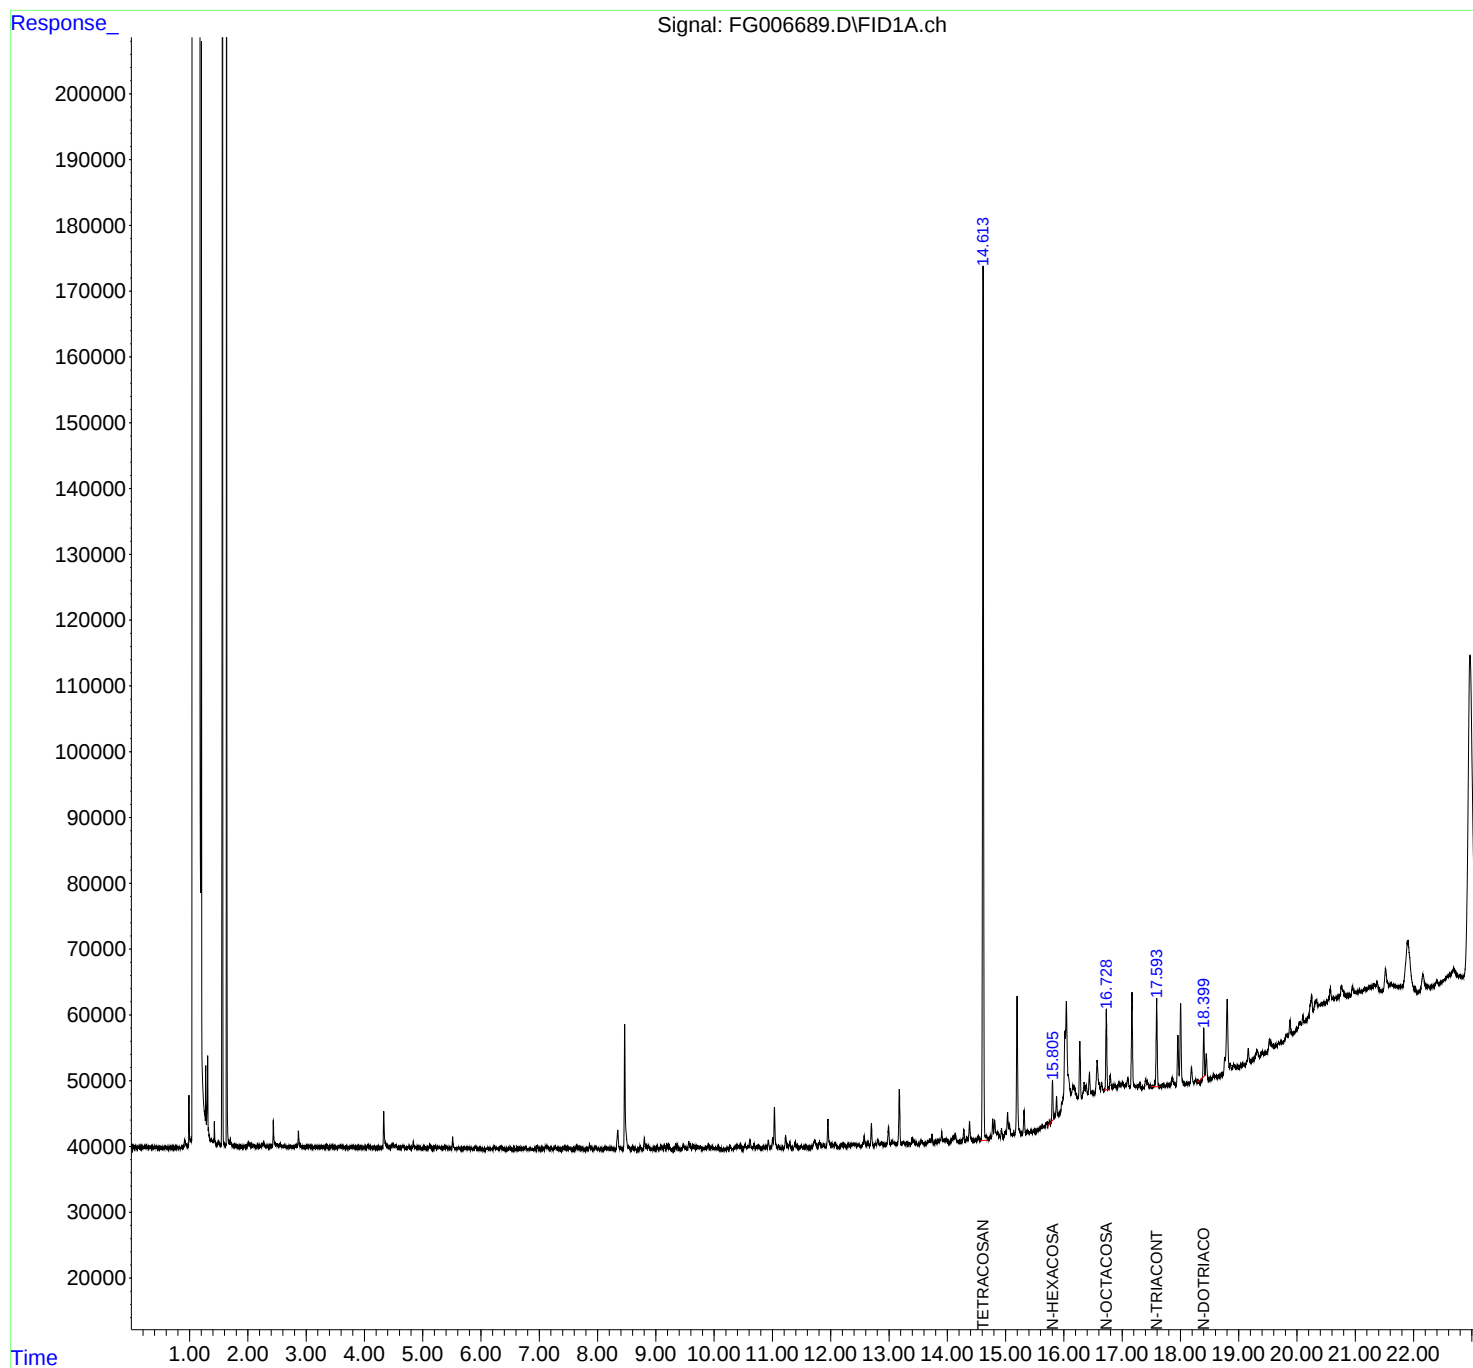


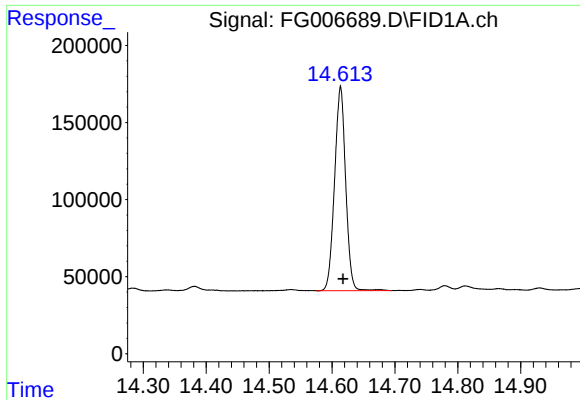

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.614 min
Delta R.T.: -0.004 min
Response: 1624908
Conc: 15.96 ug/ml

Instrument :
FID_G
ClientSampleId :

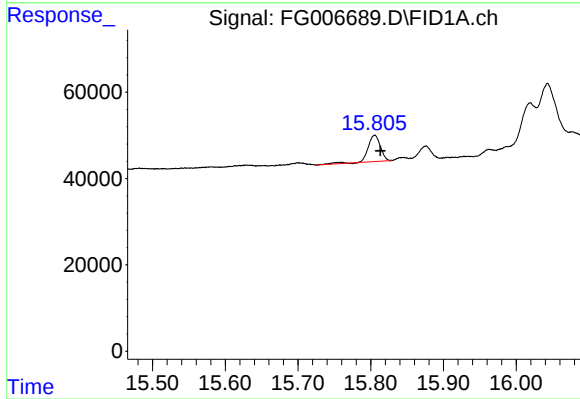


#11 N-HEXACOSANE

R.T.: 15.805 min
Delta R.T.: -0.008 min
Response: 72650
Conc: 0.63 ug/ml

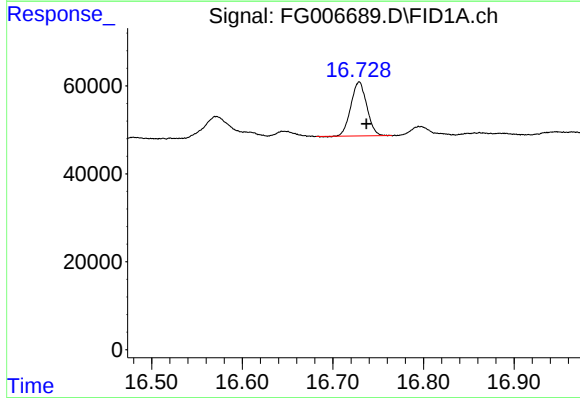


#12 N-OCTACOSANE

R.T.: 16.729 min
Delta R.T.: -0.008 min
Response: 149211
Conc: 1.27 ug/ml

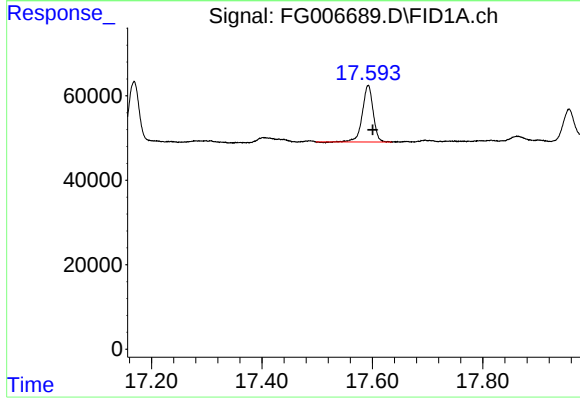

#13 N-TRIACONTANE

R.T.: 17.592 min
Delta R.T.: -0.008 min
Response: 181188
Conc: 1.51 ug/ml

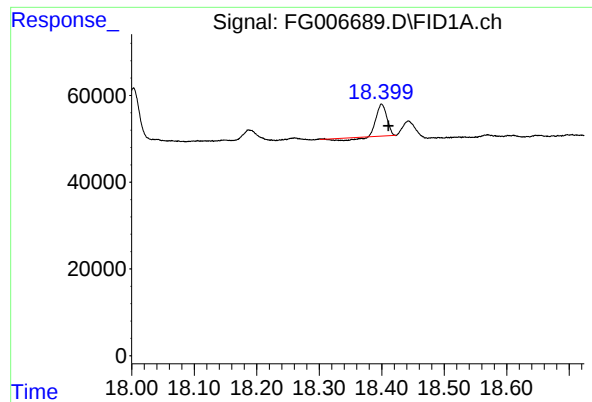

#14 N-DOTRIACONTANE

R.T.: 18.400 min
Delta R.T.: -0.010 min
Response: 74539
Conc: 0.67 ug/ml

Instrument :
FID_G
ClientSampleId :