

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
Data File : FG006692.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2020 16:32
Operator : DD\AJ
Sample : L1491-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 02:30:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.613	1642136	16.134 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.805	80905	0.696 ug/ml
12) N-OCTACOSANE	16.729	113826	0.967 ug/ml
13) N-TRIACONTANE	17.591	147733	1.231 ug/ml
14) N-DOTRIACONTANE	18.400	102613	0.923 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG0211220\
Data File : FG006692.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2020 16:32
Operator : DD\AJ
Sample : L1491-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 02:30:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

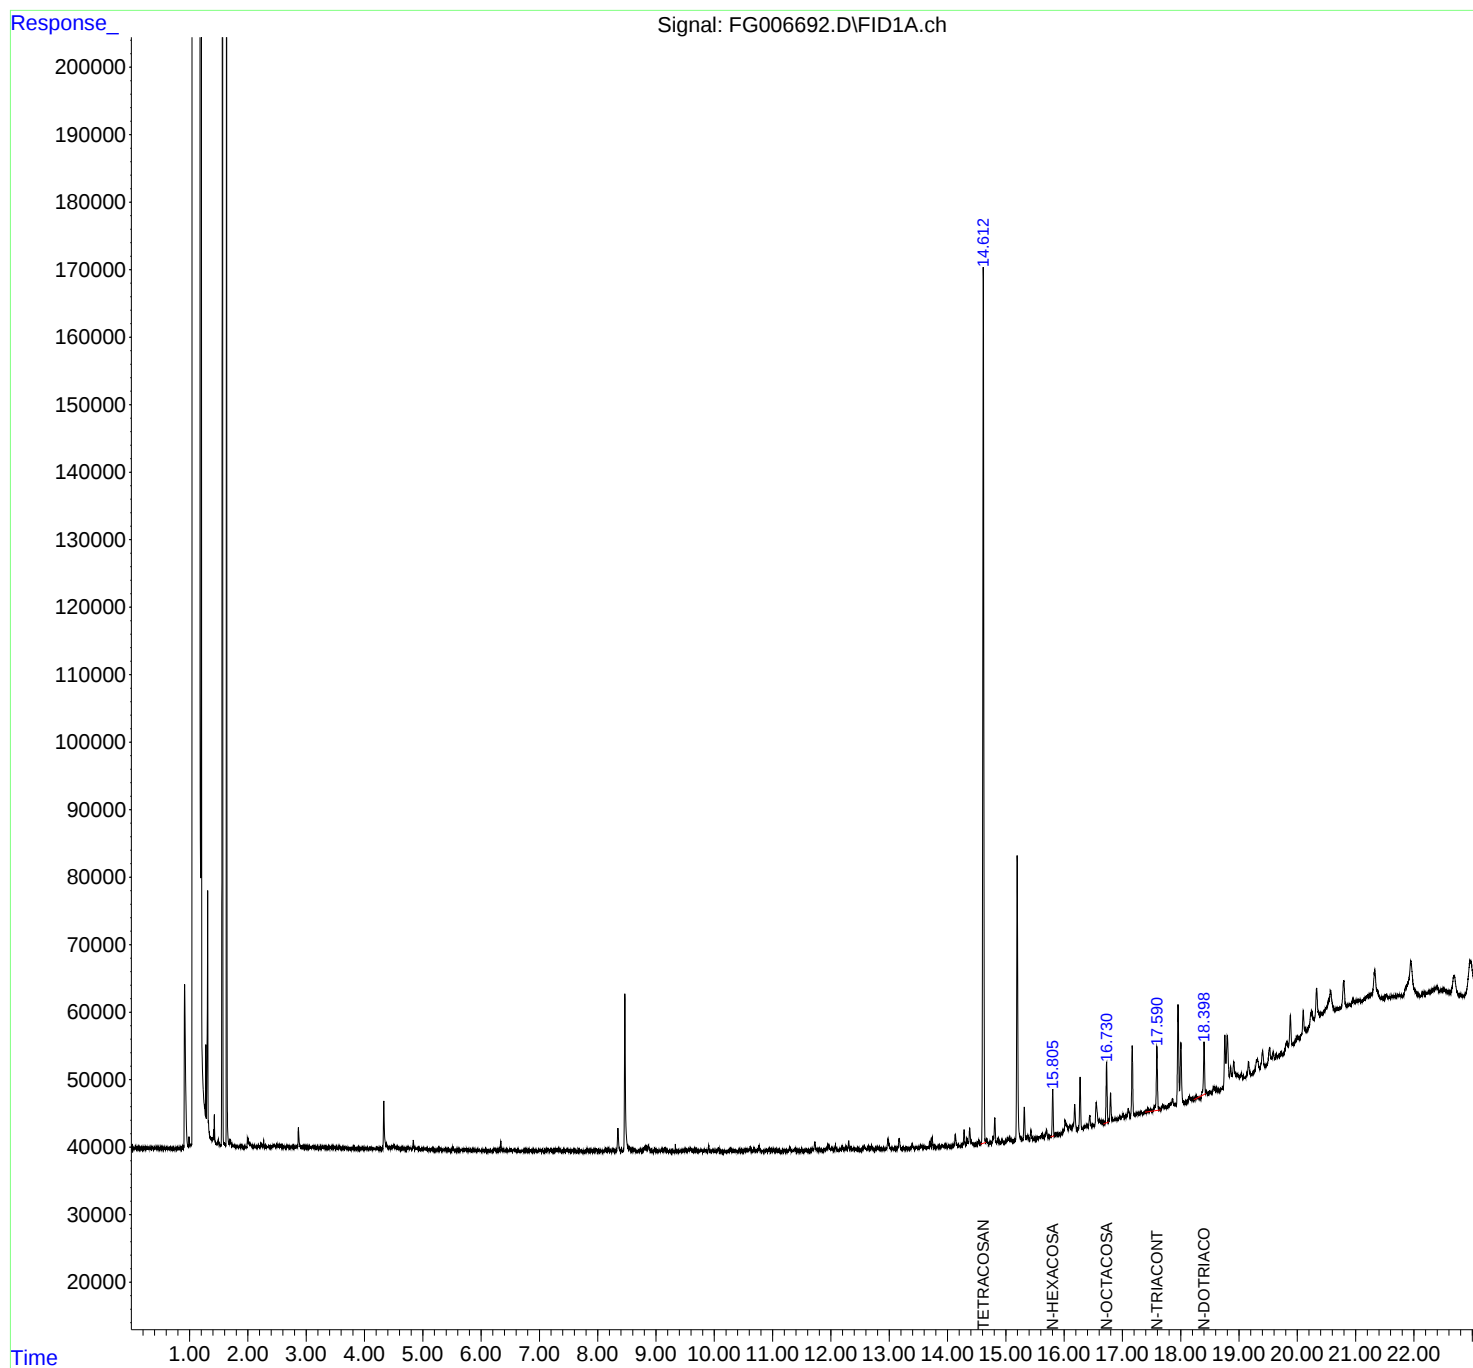


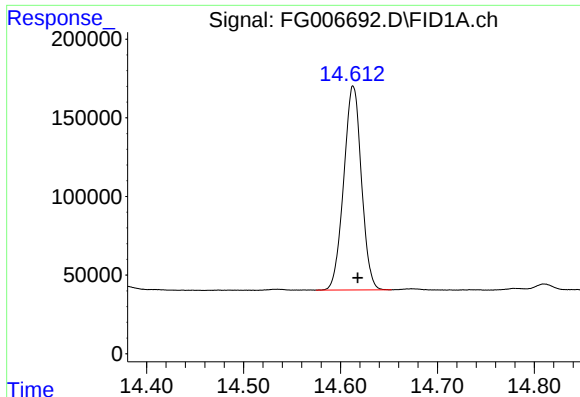

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.613 min
Delta R.T.: -0.005 min
Response: 1642136
Conc: 16.13 ug/ml

Instrument :
FID_G
ClientSampleId :

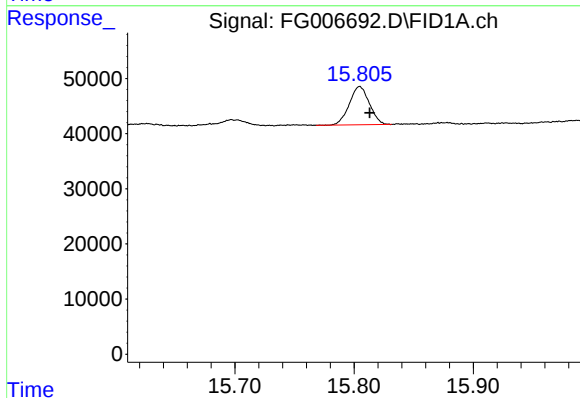


#11 N-HEXACOSANE

R.T.: 15.805 min
Delta R.T.: -0.008 min
Response: 80905
Conc: 0.70 ug/ml

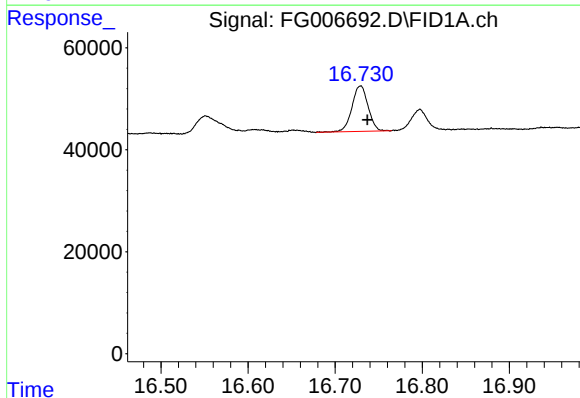


#12 N-OCTACOSANE

R.T.: 16.729 min
Delta R.T.: -0.008 min
Response: 113826
Conc: 0.97 ug/ml

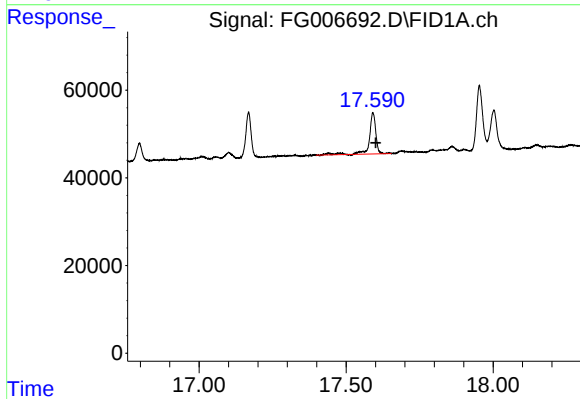

#13 N-TRIACONTANE

R.T.: 17.591 min
Delta R.T.: -0.009 min
Response: 147733
Conc: 1.23 ug/ml

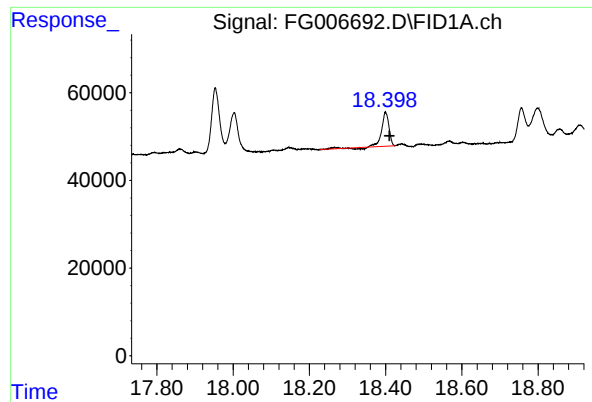

#14 N-DOTRIACONTANE

R.T.: 18.400 min
Delta R.T.: -0.010 min
Response: 102613
Conc: 0.92 ug/ml

Instrument :
FID_G
ClientSampleId :