

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
Data File : FG006697.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2020 19:03
Operator : DD\AJ
Sample : PB126763BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB126763BL

Integration File: autoint1.e
Quant Time: Feb 13 02:35:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	1624166	15.958 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021220\
Data File : FG006697.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2020 19:03
Operator : DD\AJ
Sample : PB126763BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB126763BL

Integration File: autoint1.e
Quant Time: Feb 13 02:35:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

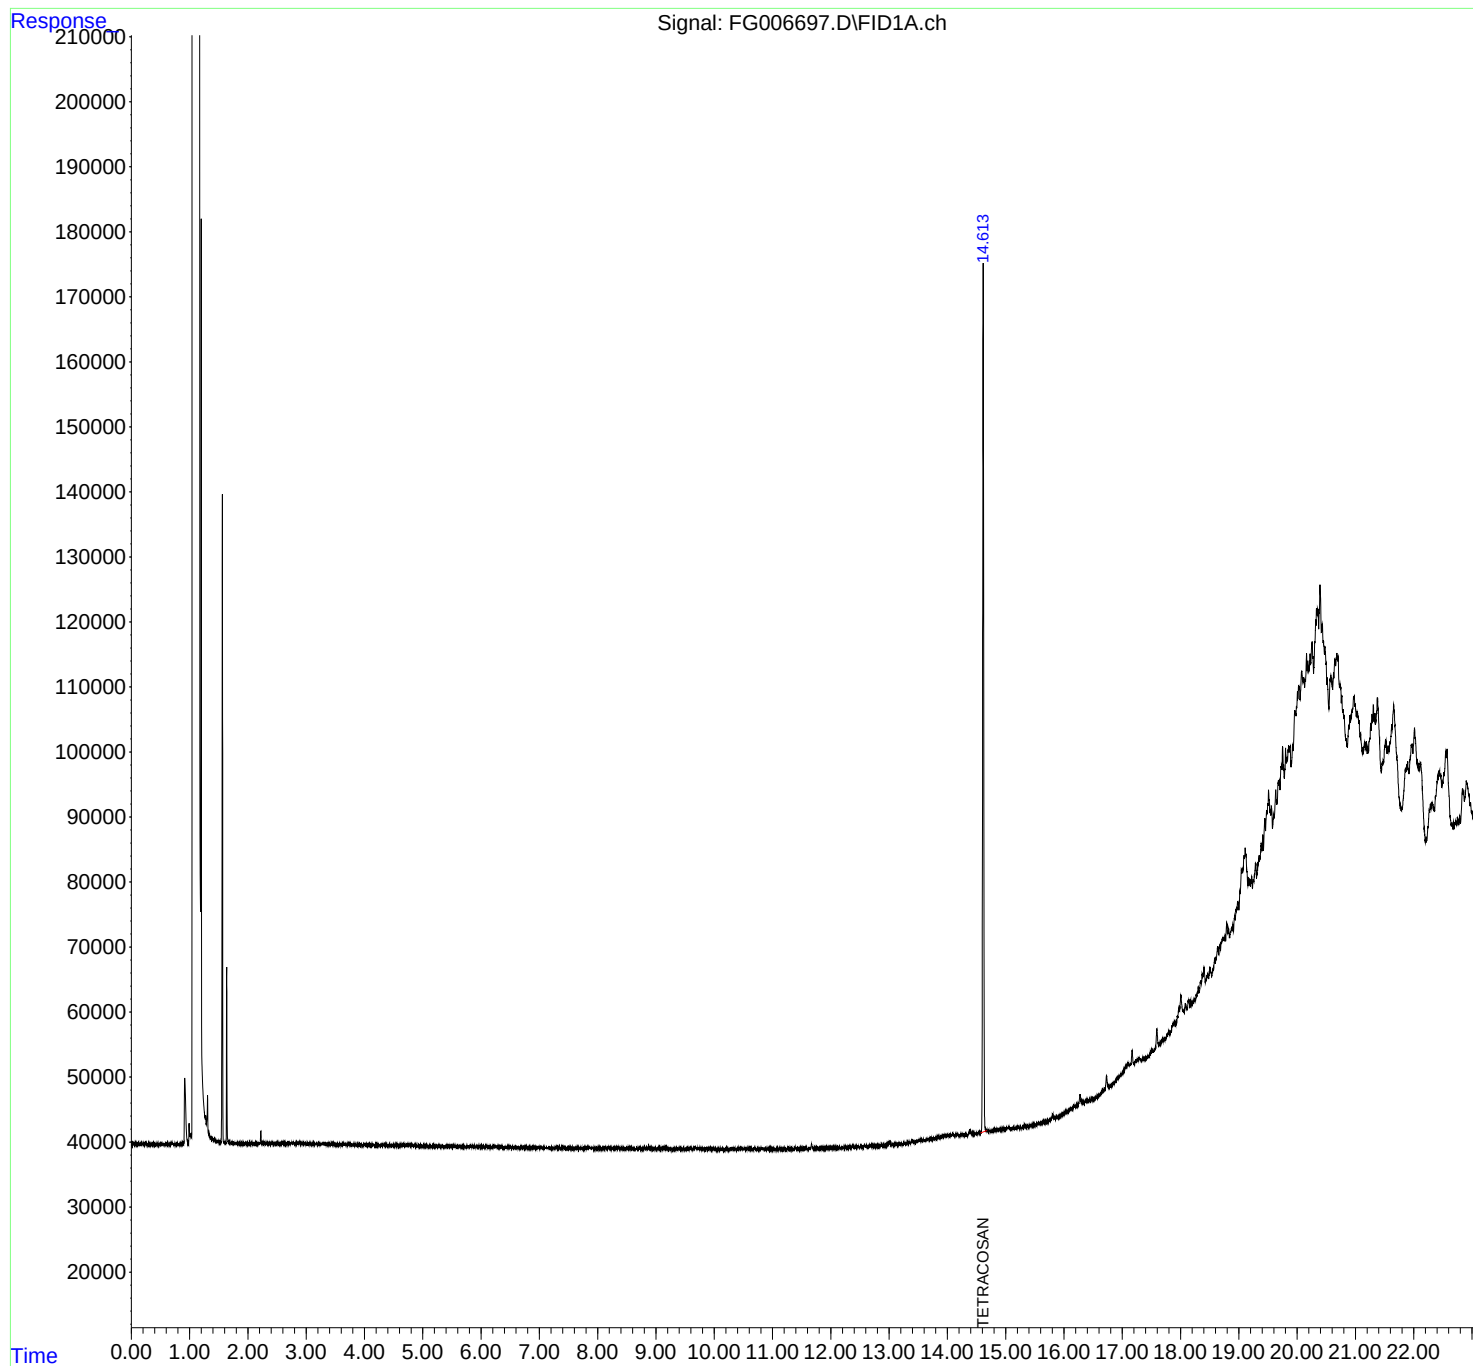

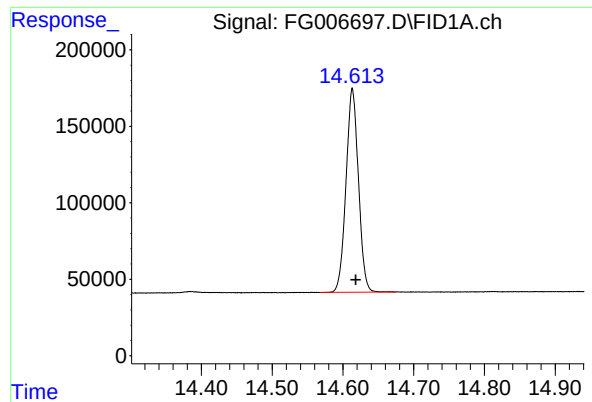

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.614 min
Delta R.T.: -0.004 min
Response: 1624166
Conc: 15.96 ug/ml

Instrument :
FID_G
ClientSampleId :
PB126763BL