

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021224AL\
 Data File : FG013488.D
 Signal(s) : FID1A.ch
 Acq On : 12 Feb 2024 13:55
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 12 22:41:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 021224.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 12 22:40:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.998	84096	0.743 ug/ml
20) T n-Hexatriacontane (C36)	20.554	40176	0.386 ug/ml
22) T n-Tetracontane (C40)	22.258f	98789	0.967 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021224AL\
Data File : FG013488.D
Signal(s) : FID1A.ch
Acq On : 12 Feb 2024 13:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 12 22:41:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 021224.M
Quant Title : GC Extractables
QLast Update : Mon Feb 12 22:40:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

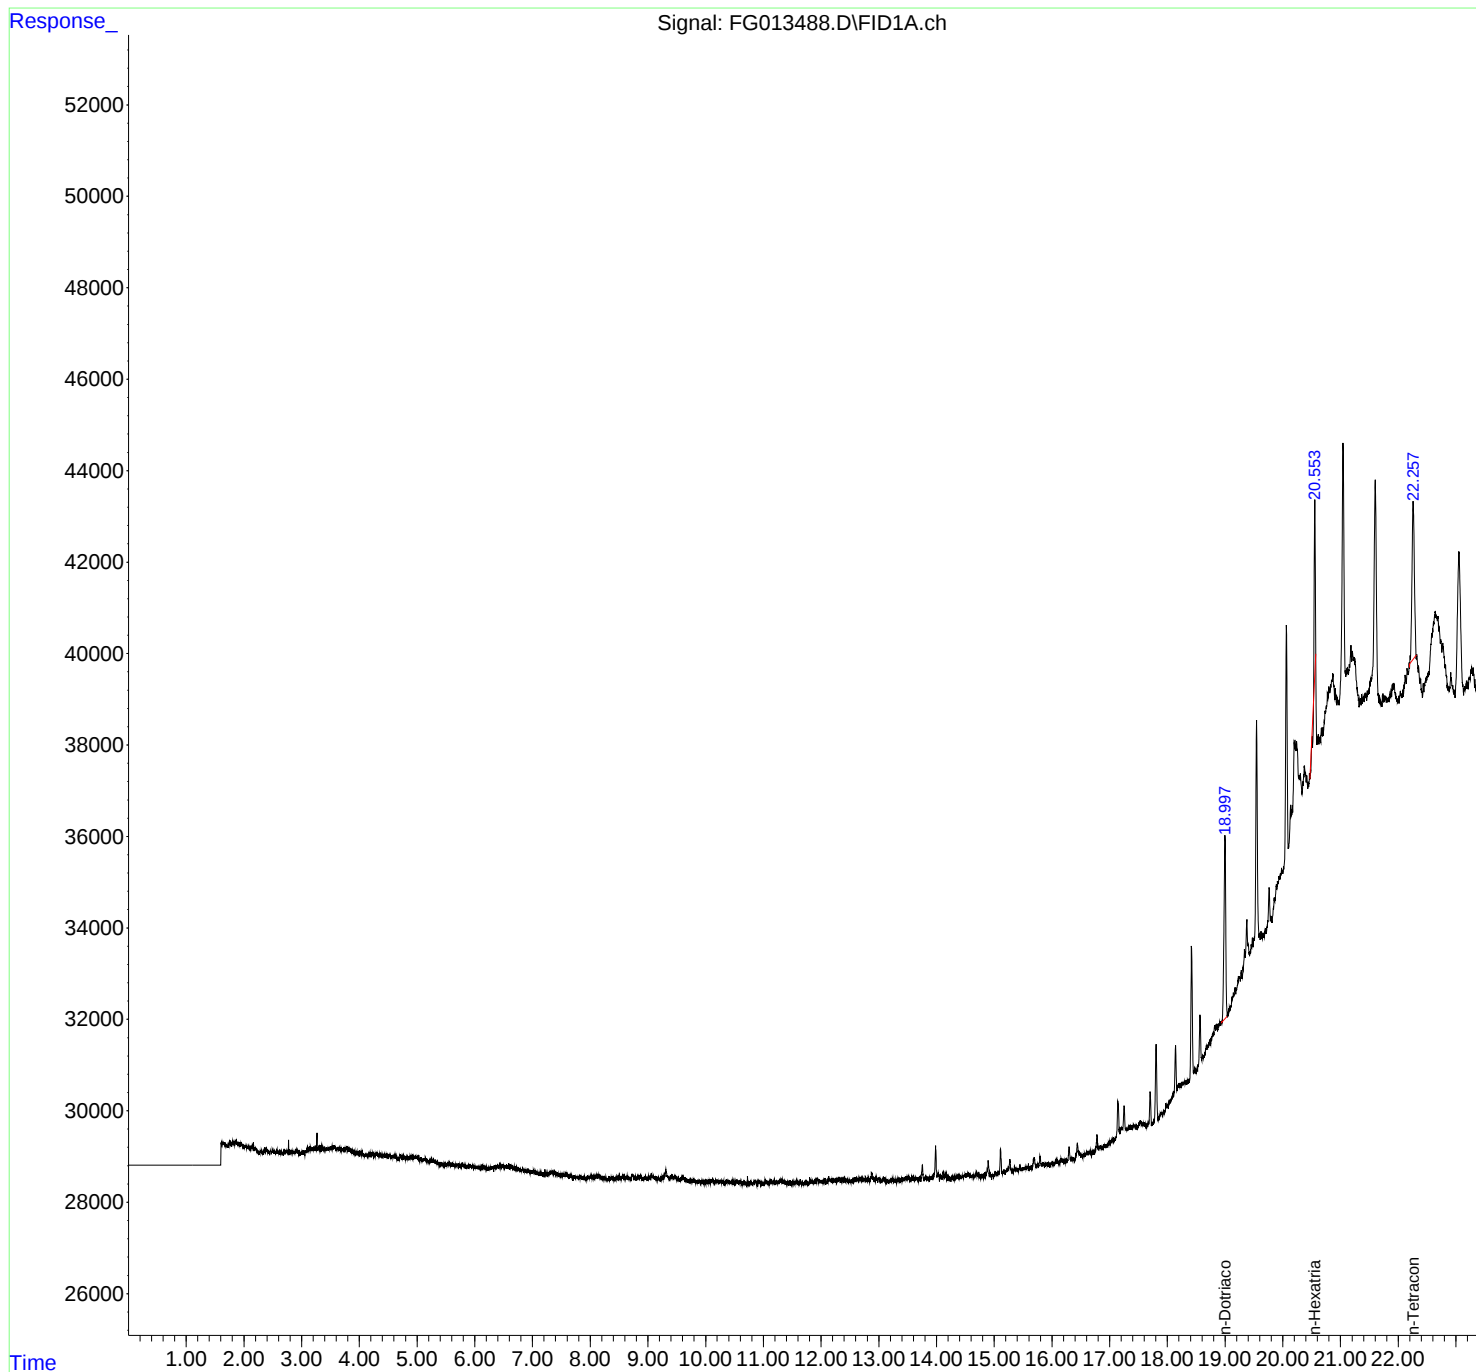


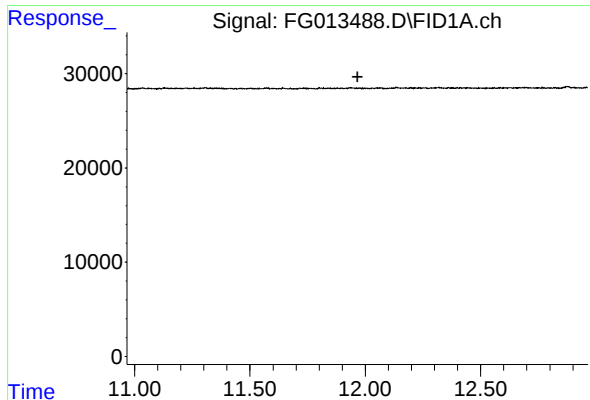

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.966 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

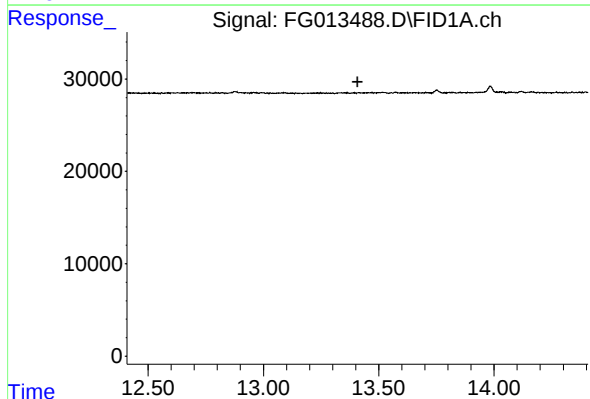


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.408 min
Response: 0
Conc: N.D.

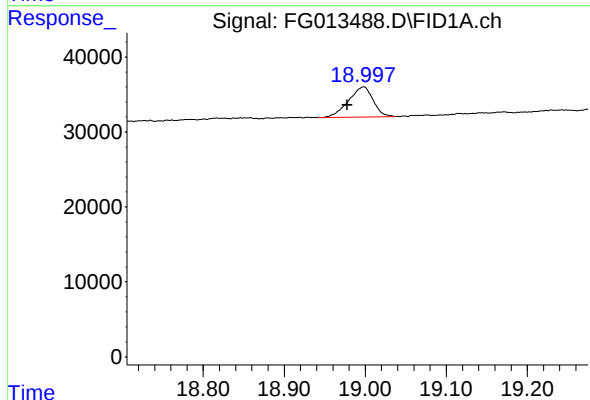


#18 n-Dotriacontane (C32)

R.T.: 18.998 min
Delta R.T.: 0.020 min
Response: 84096
Conc: 0.74 ug/ml

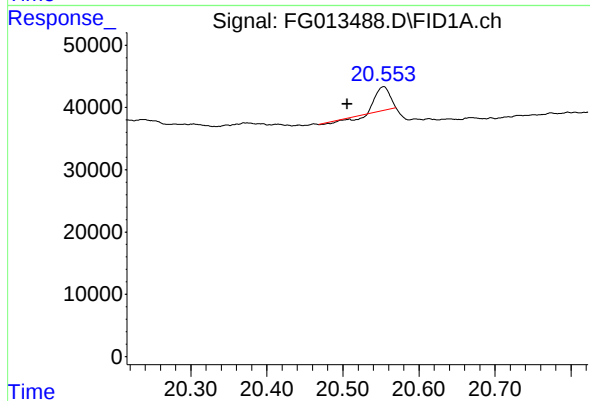

#20 n-Hexatriacontane (C36)

R.T.: 20.554 min
Delta R.T.: 0.048 min
Response: 40176
Conc: 0.39 ug/ml

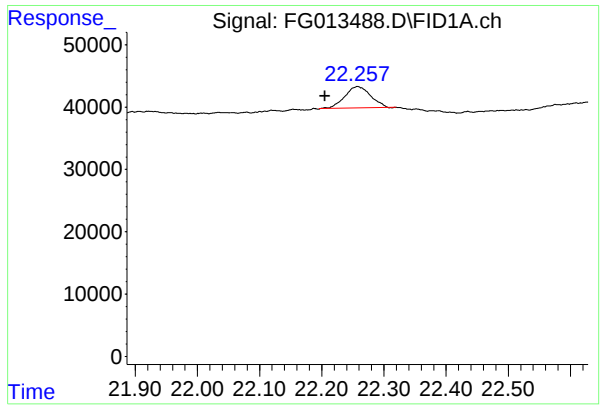

#22 n-Tetracontane (C40)

R.T.: 22.258 min
Delta R.T.: 0.053 min
Response: 98789
Conc: 0.97 ug/ml

Instrument :

FID_G

ClientSampleId :