

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021319\
 Data File : FG003787.D
 Signal(s) : FID1A.ch
 Acq On : 13 Feb 2019 14:35
 Operator : AJ\SJ
 Sample : K1343-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 14 00:25:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.212	211682	1.341 ug/ml
4) N-TETRADECANE	8.005	395547	2.506 ug/ml
5) N-HEXADECANE	9.605	489930	3.110 ug/ml
6) N-OCTADECANE	11.047	347227	2.206 ug/ml
7) N-EICOSANE	12.359	228372	1.458 ug/ml
8) N-DOCOSANE	13.559	159050	1.029 ug/ml
12) N-OCTACOSANE	16.636	92864	0.645 ug/ml
13) N-TRIACONTANE	17.523	309962	2.190 ug/ml
14) N-DOTRIACONTANE	18.357	361790	2.763 ug/ml
15) N-TETRATRIACONTANE	19.144	360354	3.055 ug/ml
16) N-HEXATRIACONTANE	19.887	159583	1.512 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021319\
Data File : FG003787.D
Signal(s) : FID1A.ch
Acq On : 13 Feb 2019 14:35
Operator : AJ\SJ
Sample : K1343-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 14 00:25:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

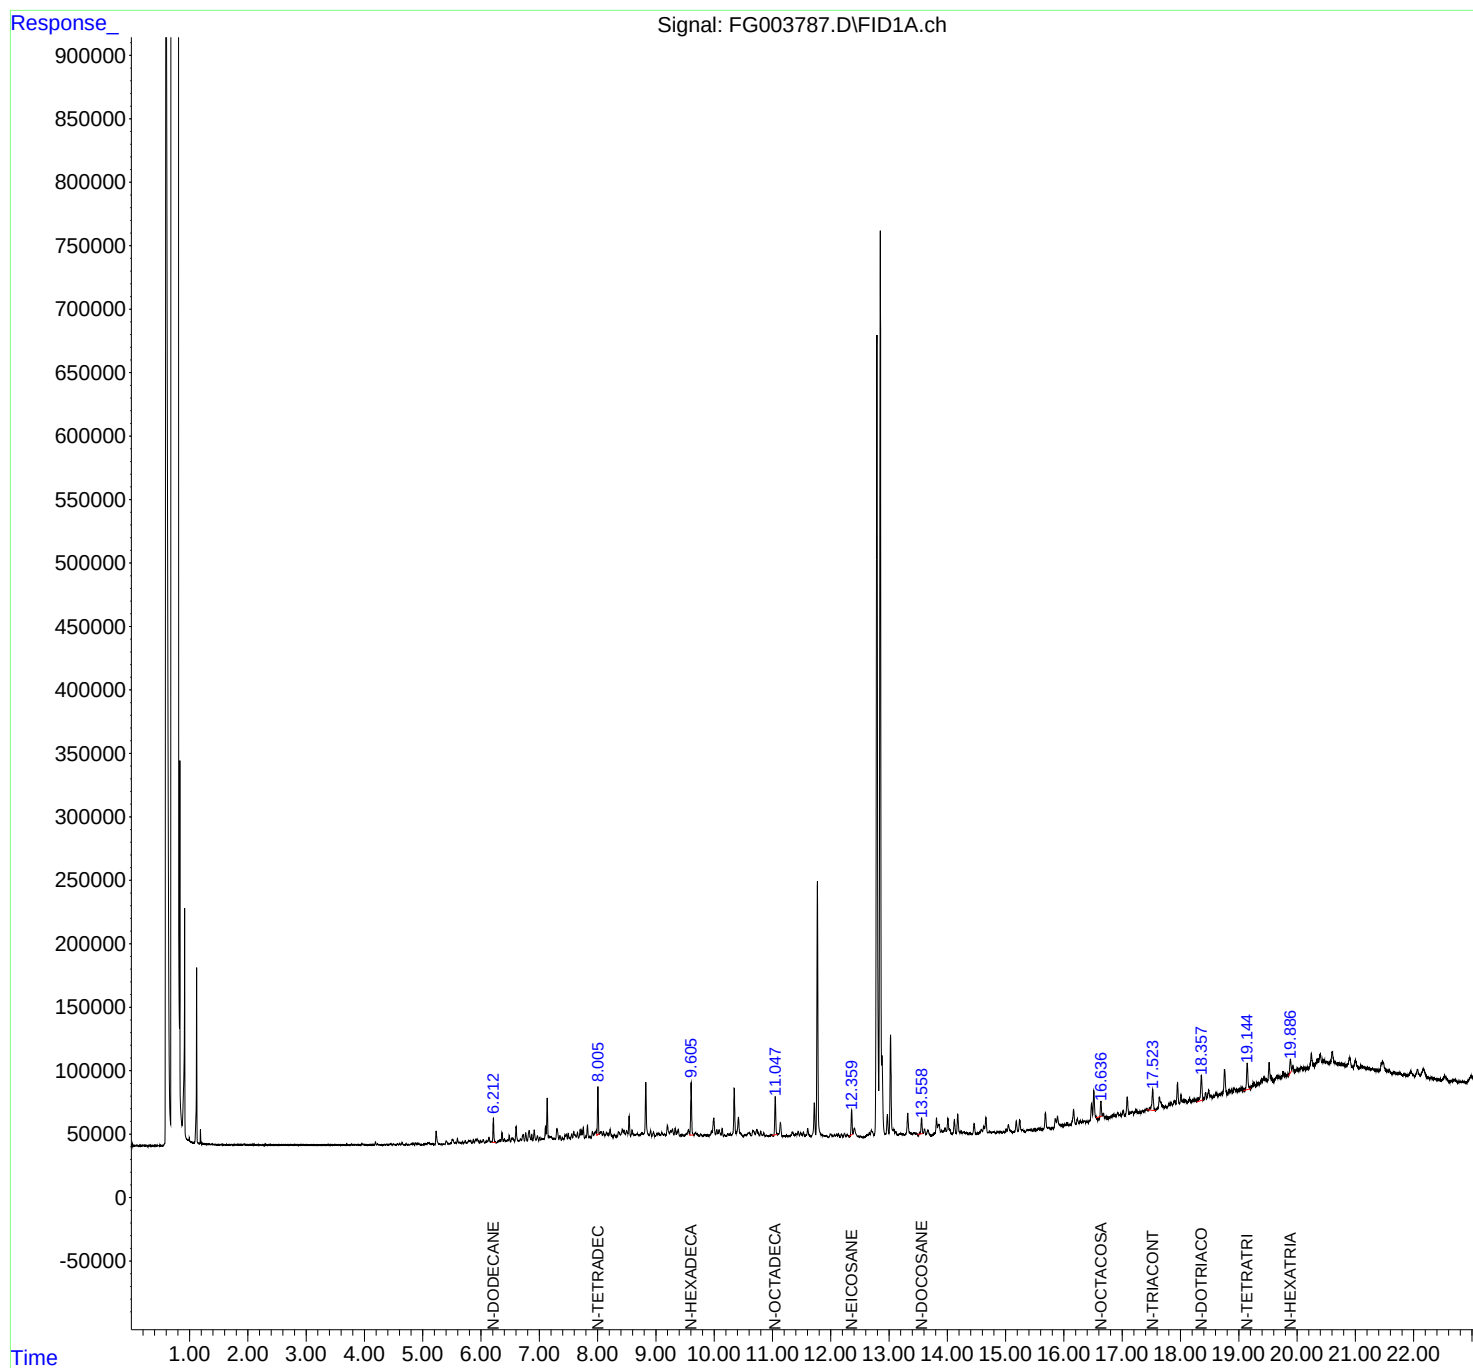

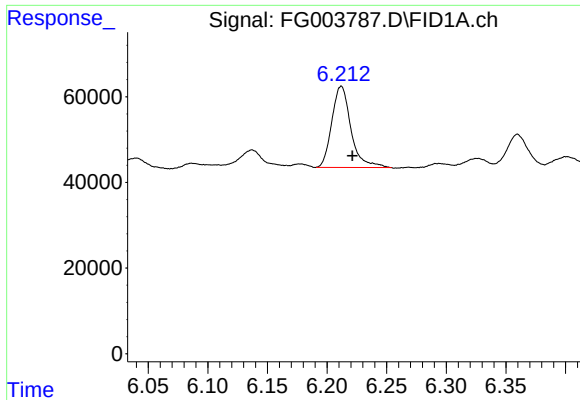


#3 N-DODECANE

R.T.: 6.212 min
Delta R.T.: -0.009 min
Response: 211682
Conc: 1.34 ug/ml

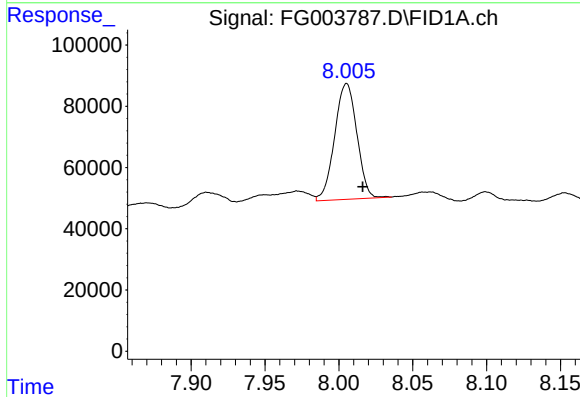


#4 N-TETRADECANE

R.T.: 8.005 min
Delta R.T.: -0.011 min
Response: 395547
Conc: 2.51 ug/ml

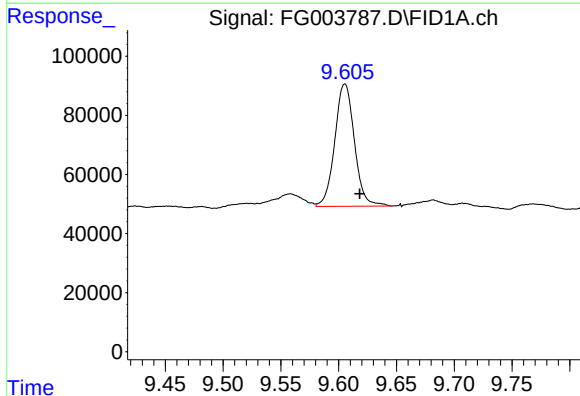


#5 N-HEXADECANE

R.T.: 9.605 min
Delta R.T.: -0.013 min
Response: 489930
Conc: 3.11 ug/ml

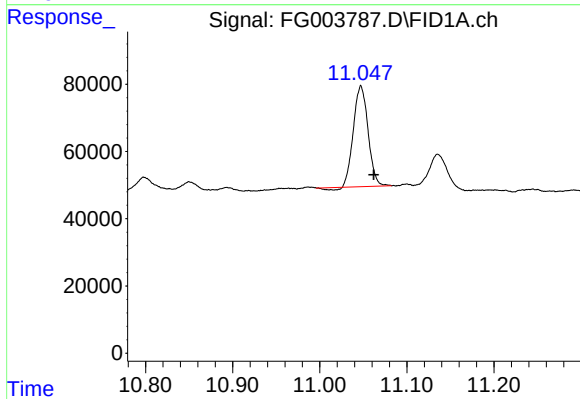


#6 N-OCTADECANE

R.T.: 11.047 min
Delta R.T.: -0.015 min
Response: 347227
Conc: 2.21 ug/ml

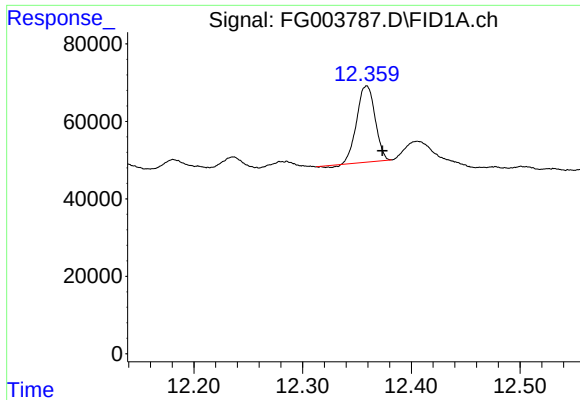


#7 N-EICOSANE

R.T.: 12.359 min
Delta R.T.: -0.015 min
Response: 228372
Conc: 1.46 ug/ml

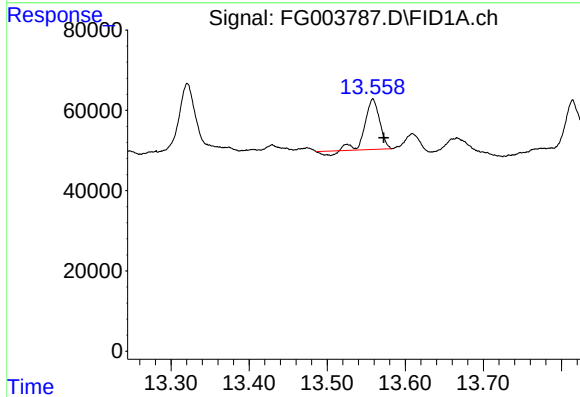


#8 N-DOCOSANE

R.T.: 13.559 min
Delta R.T.: -0.014 min
Response: 159050
Conc: 1.03 ug/ml

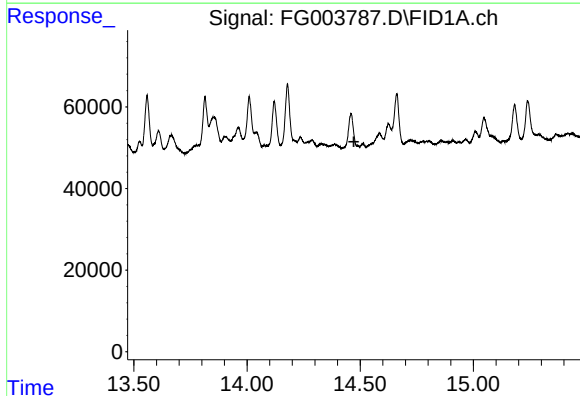


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.472 min
Response: 0
Conc: N.D.

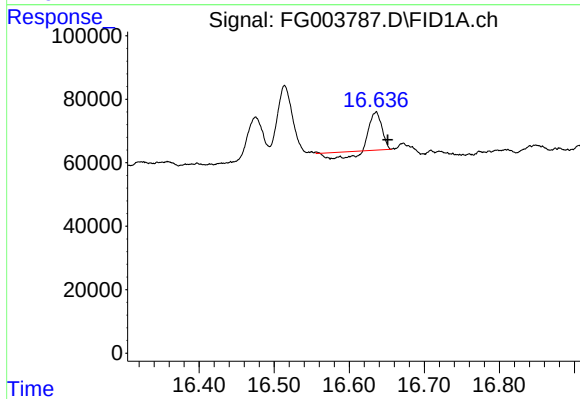


#12 N-OCTACOSANE

R.T.: 16.636 min
Delta R.T.: -0.016 min
Response: 92864
Conc: 0.64 ug/ml

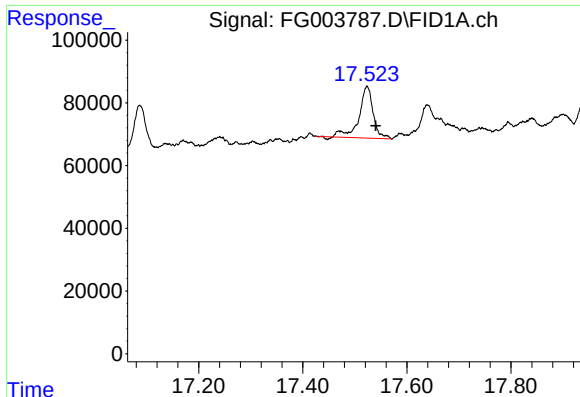


#13 N-TRIACONTANE

R.T.: 17.523 min
Delta R.T.: -0.017 min
Response: 309962
Conc: 2.19 ug/ml

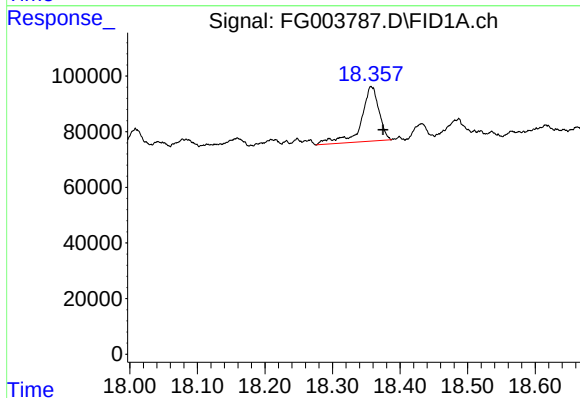


#14 N-DOTRIACONTANE

R.T.: 18.357 min
Delta R.T.: -0.018 min
Response: 361790
Conc: 2.76 ug/ml

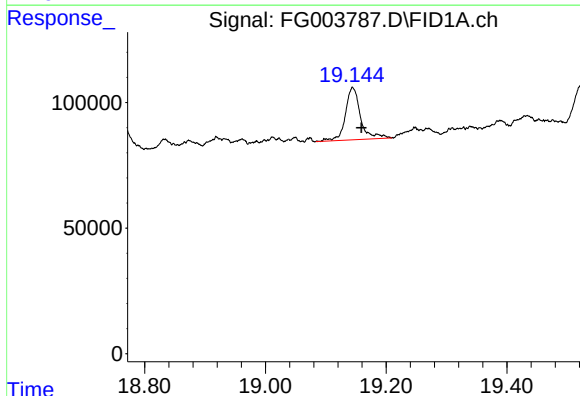

#15 N-TETRATRIACONTANE

R.T.: 19.144 min
Delta R.T.: -0.015 min
Response: 360354
Conc: 3.06 ug/ml

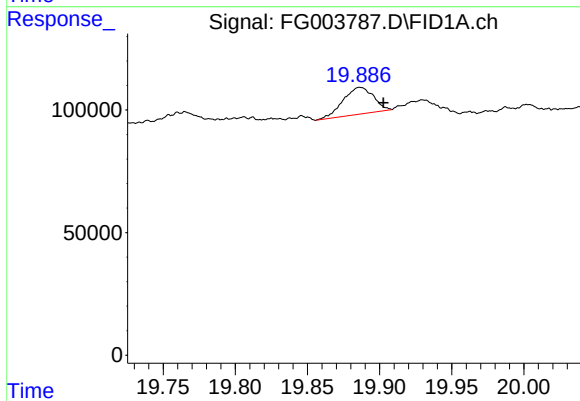

#16 N-HEXATRIACONTANE

R.T.: 19.887 min
Delta R.T.: -0.016 min
Response: 159583
Conc: 1.51 ug/ml