

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021319\
Data File : FG003790.D
Signal(s) : FID1A.ch
Acq On : 13 Feb 2019 16:06
Operator : AJ\SJ
Sample : K1343-07 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 14 00:26:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
4) N-TETRADECANE	8.005	163388	1.035 ug/ml
5) N-HEXADECANE	9.605	171860	1.091 ug/ml
7) N-EICOSANE	12.398	1141552	7.289 ug/ml
10) N-TETRACOSANE	14.620f	348185	2.311 ug/ml
12) N-OCTACOSANE	16.635	187223	1.300 ug/ml
13) N-TRIACONTANE	17.523	273430	1.932 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021319\
Data File : FG003790.D
Signal(s) : FID1A.ch
Acq On : 13 Feb 2019 16:06
Operator : AJ\SJ
Sample : K1343-07 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 14 00:26:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

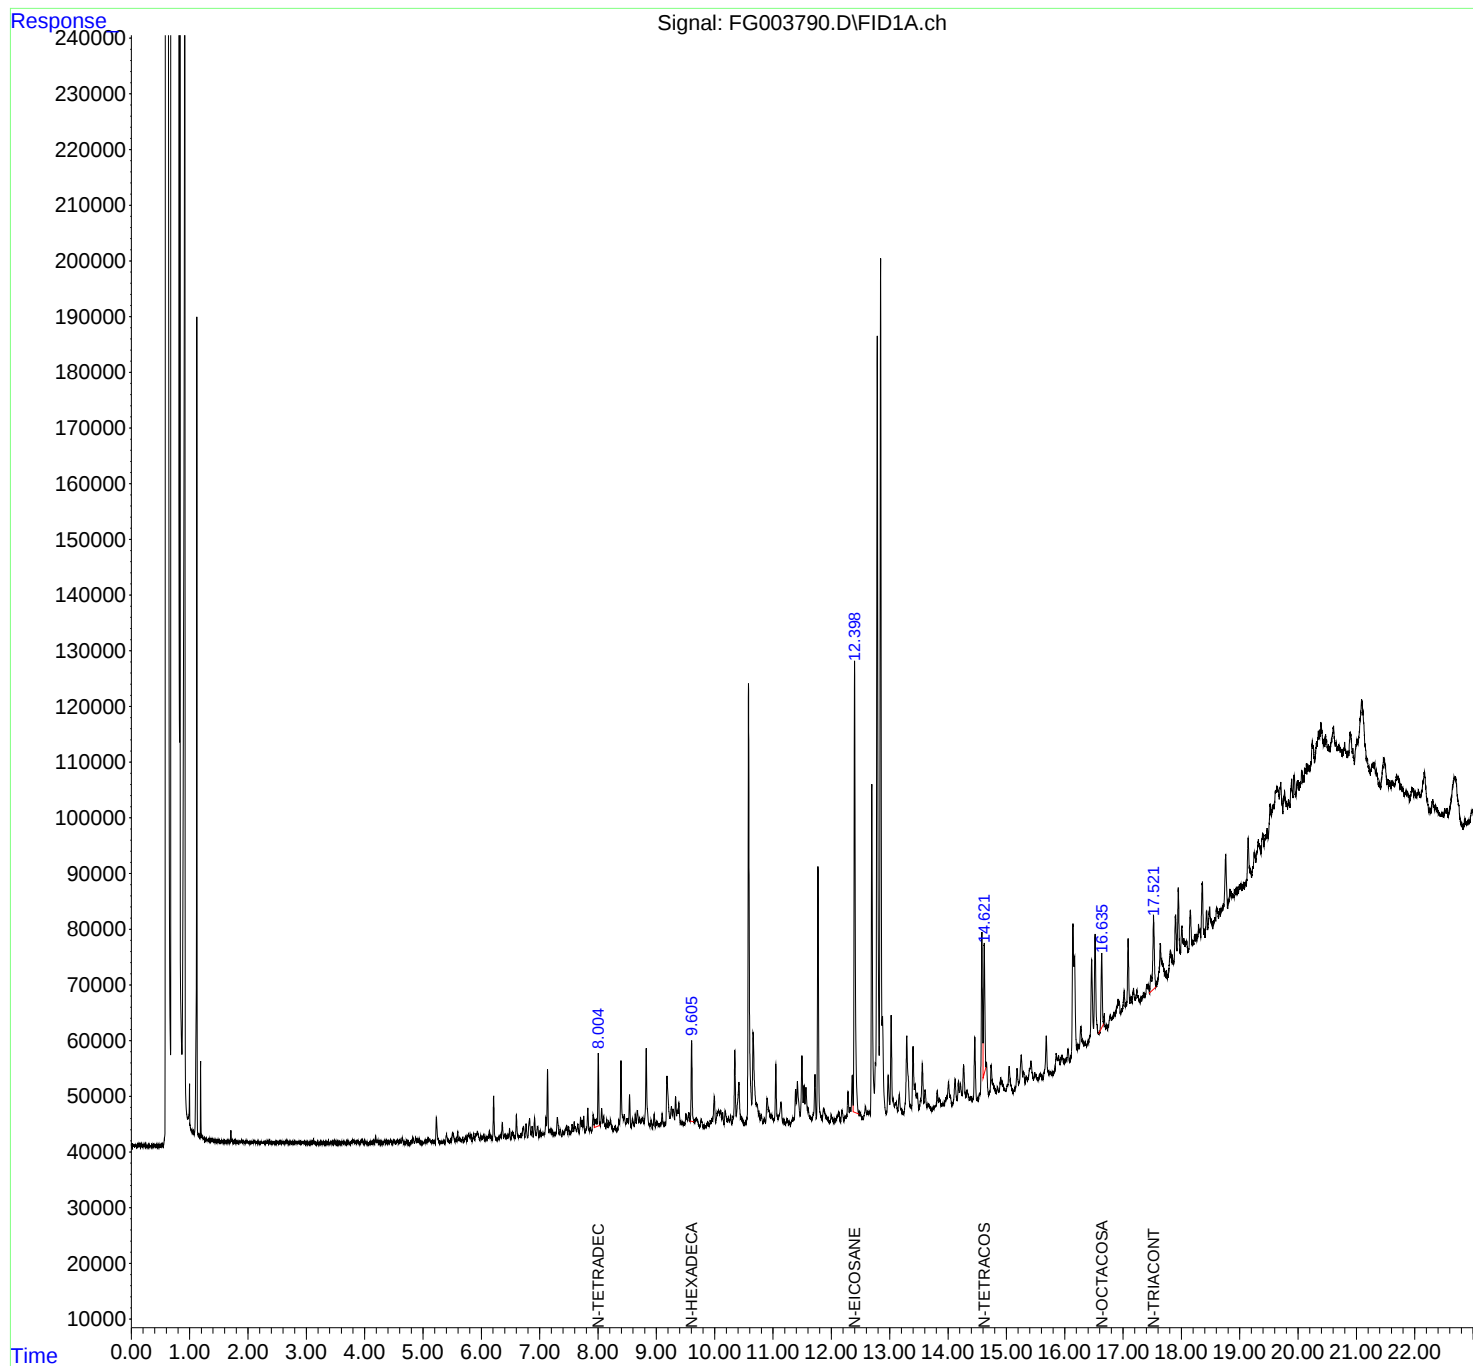

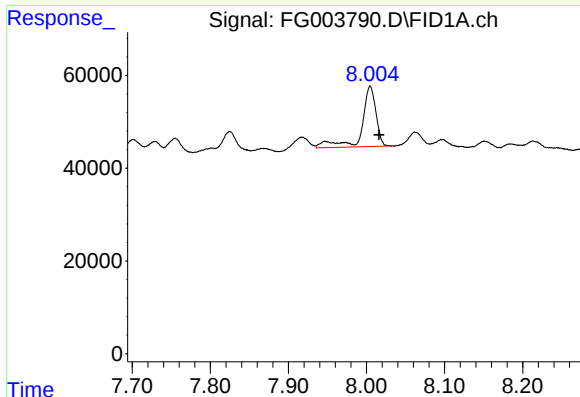


#4 N-TETRADECANE

R.T.: 8.005 min
Delta R.T.: -0.011 min
Response: 163388
Conc: 1.04 ug/ml

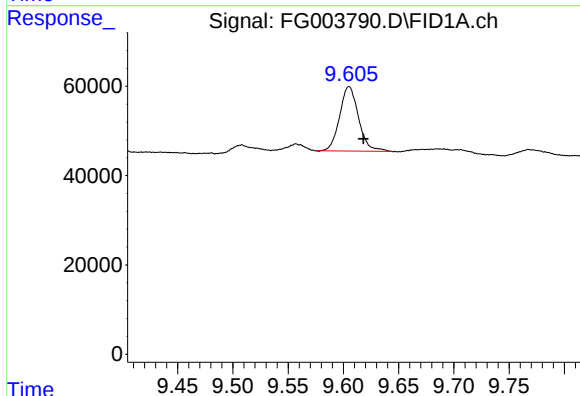


#5 N-HEXADECANE

R.T.: 9.605 min
Delta R.T.: -0.013 min
Response: 171860
Conc: 1.09 ug/ml

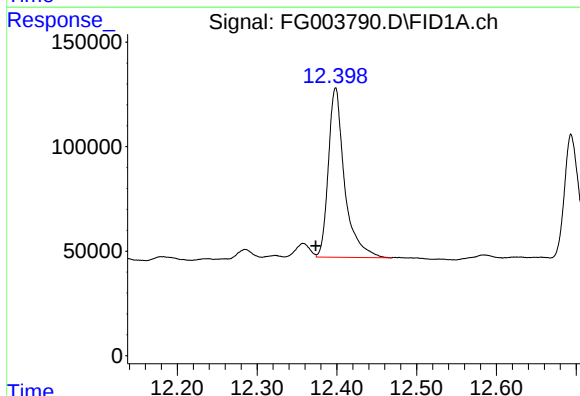


#7 N-EICOSANE

R.T.: 12.398 min
Delta R.T.: 0.025 min
Response: 1141552
Conc: 7.29 ug/ml

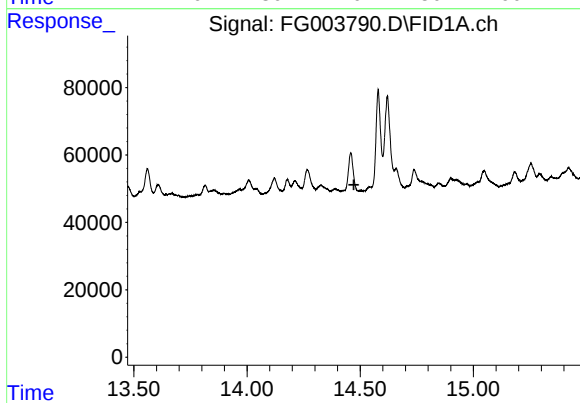


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.472 min
Response: 0
Conc: N.D.

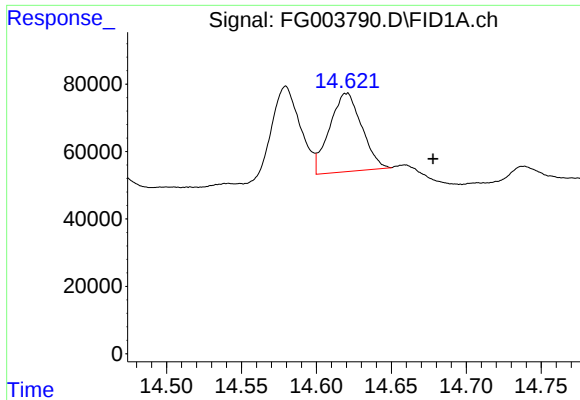


#10 N-TETRACOSANE

R.T.: 14.620 min
Delta R.T.: -0.058 min
Response: 348185
Conc: 2.31 ug/ml

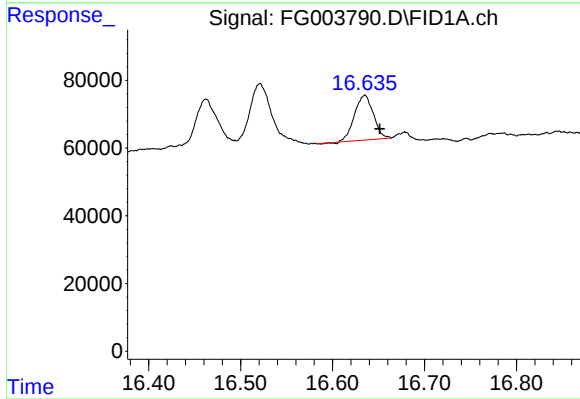

#12 N-OCTACOSANE

R.T.: 16.635 min
Delta R.T.: -0.016 min
Response: 187223
Conc: 1.30 ug/ml

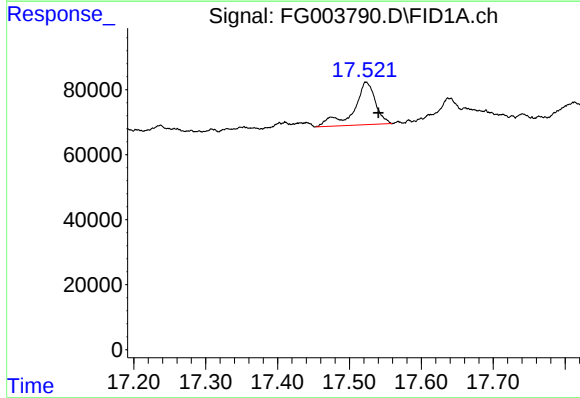

#13 N-TRIACONTANE

R.T.: 17.523 min
Delta R.T.: -0.017 min
Response: 273430
Conc: 1.93 ug/ml