

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021319\
 Data File : FG003798.D
 Signal(s) : FID1A.ch
 Acq On : 13 Feb 2019 20:10
 Operator : AJ\SJ
 Sample : K1343-19 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 14 00:28:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.212	438387	2.777 ug/ml
4) N-TETRADECANE	8.006	650346	4.121 ug/ml
5) N-HEXADECANE	9.606	850189	5.397 ug/ml
6) N-OCTADECANE	11.049	715274	4.544 ug/ml
7) N-EICOSANE	12.360	515367	3.291 ug/ml
8) N-DOCOSANE	13.560	291896	1.888 ug/ml
10) N-TETRACOSANE	14.663	420595	2.791 ug/ml
11) N-HEXACOSANE	15.686	378982	2.576 ug/ml
12) N-OCTACOSANE	16.639	391517	2.717 ug/ml
13) N-TRIACONTANE	17.526	573328	4.051 ug/ml
14) N-DOTRIACONTANE	18.361	534312	4.080 ug/ml
15) N-TETRATRIACONTANE	19.148	625462	5.303 ug/ml
16) N-HEXATRIACONTANE	19.888	440242	4.171 ug/ml
17) N-OCTATRIACONTANE	20.610	376772	3.854 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021319\
Data File : FG003798.D
Signal(s) : FID1A.ch
Acq On : 13 Feb 2019 20:10
Operator : AJ\SJ
Sample : K1343-19 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 14 00:28:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

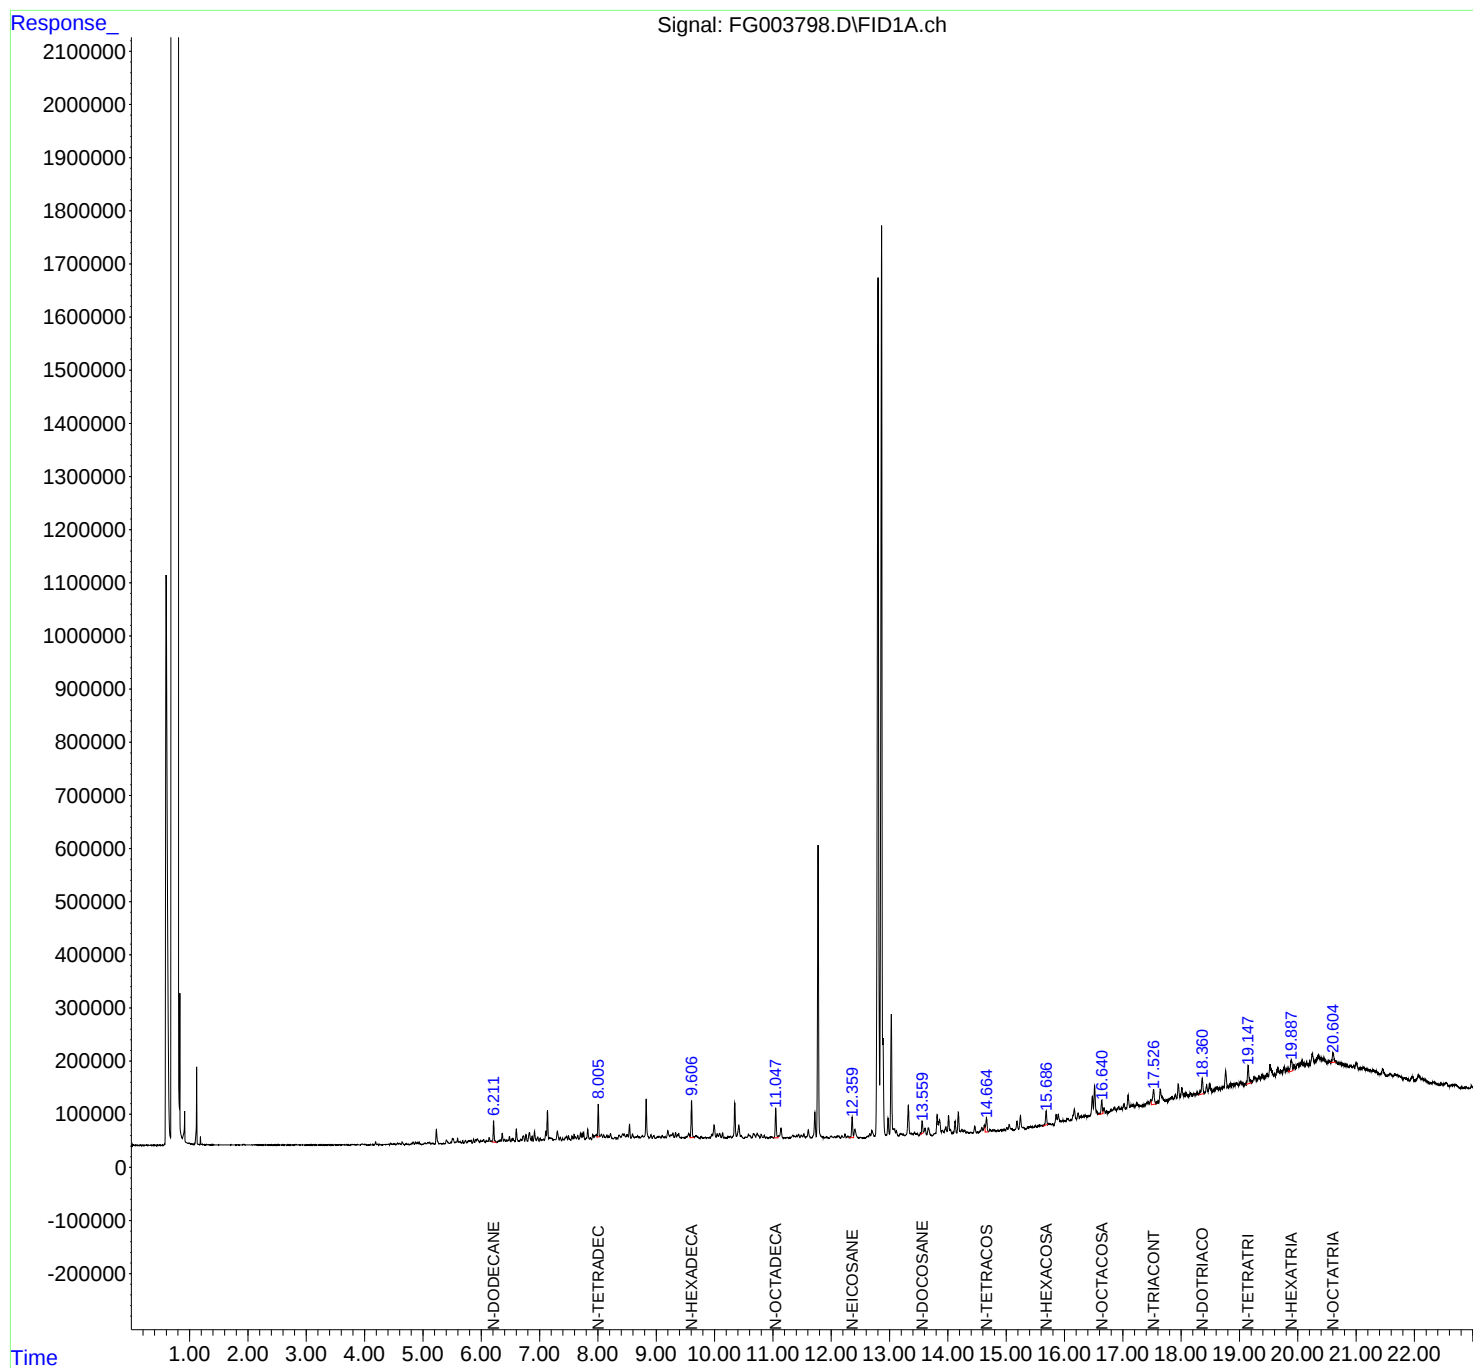

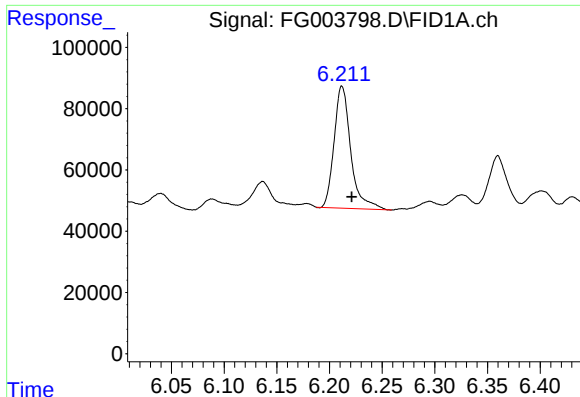


#3 N-DODECANE

R.T.: 6.212 min
Delta R.T.: -0.009 min
Response: 438387
Conc: 2.78 ug/ml

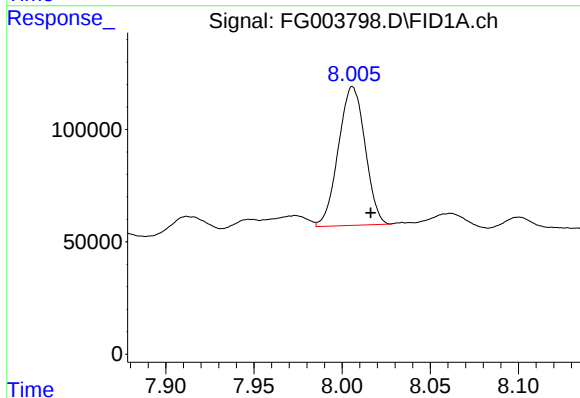


#4 N-TETRADECANE

R.T.: 8.006 min
Delta R.T.: -0.010 min
Response: 650346
Conc: 4.12 ug/ml

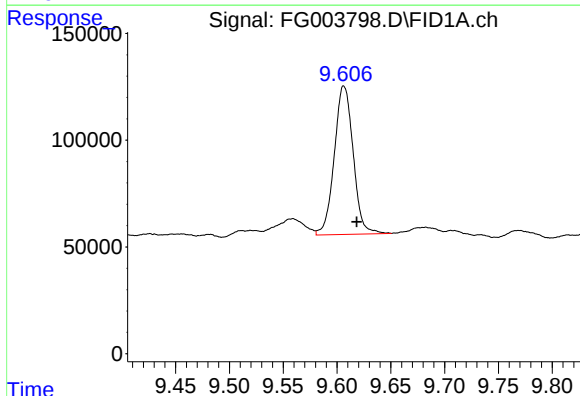


#5 N-HEXADECANE

R.T.: 9.606 min
Delta R.T.: -0.012 min
Response: 850189
Conc: 5.40 ug/ml

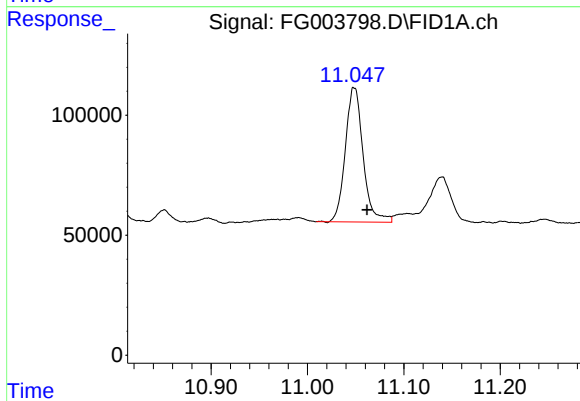


#6 N-OCTADECANE

R.T.: 11.049 min
Delta R.T.: -0.013 min
Response: 715274
Conc: 4.54 ug/ml

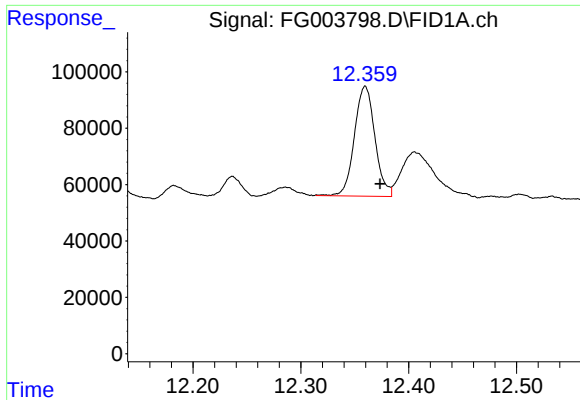


#7 N-EICOSANE

R.T.: 12.360 min
Delta R.T.: -0.014 min
Response: 515367
Conc: 3.29 ug/ml

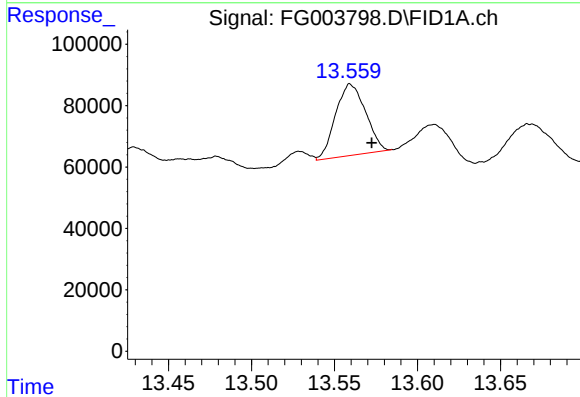


#8 N-DOCOSANE

R.T.: 13.560 min
Delta R.T.: -0.013 min
Response: 291896
Conc: 1.89 ug/ml

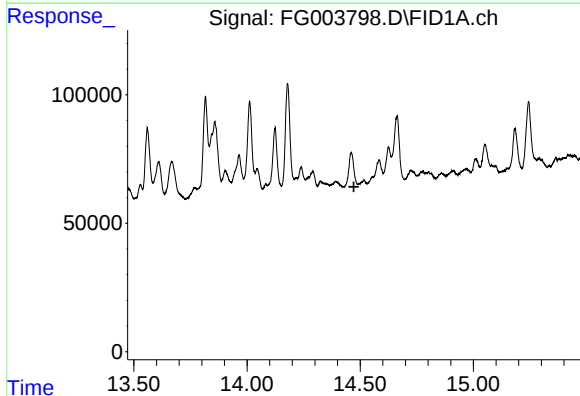


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.472 min
Response: 0
Conc: N.D.

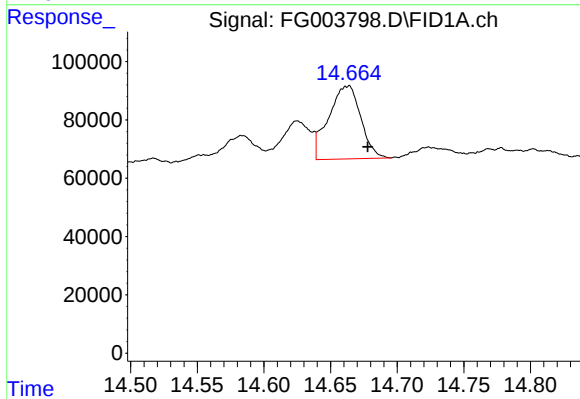


#10 N-TETRACOSANE

R.T.: 14.663 min
Delta R.T.: -0.015 min
Response: 420595
Conc: 2.79 ug/ml

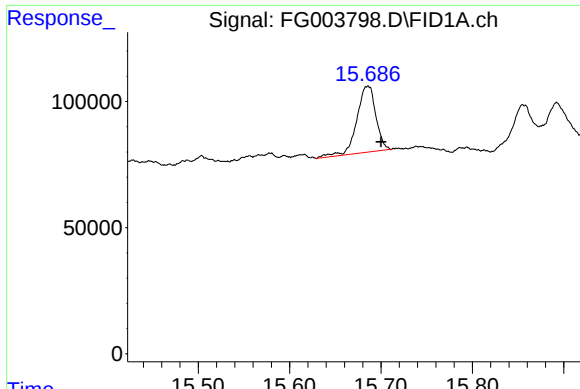


#11 N-HEXACOSANE

R.T.: 15.686 min
Delta R.T.: -0.014 min
Response: 378982
Conc: 2.58 ug/ml

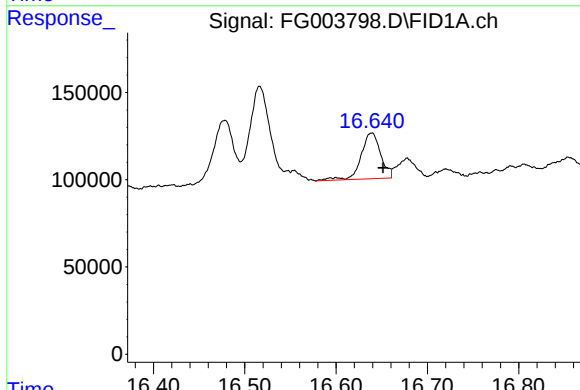


#12 N-OCTACOSANE

R.T.: 16.639 min
Delta R.T.: -0.012 min
Response: 391517
Conc: 2.72 ug/ml

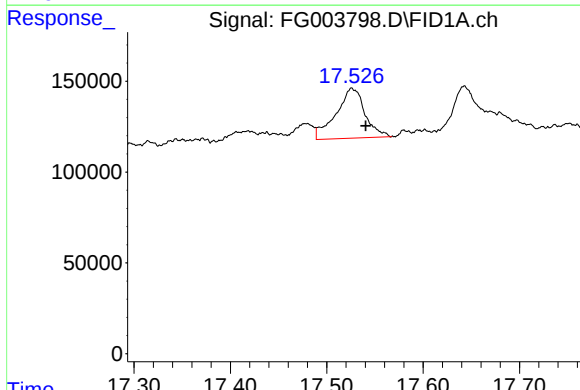


#13 N-TRIACONTANE

R.T.: 17.526 min
Delta R.T.: -0.014 min
Response: 573328
Conc: 4.05 ug/ml

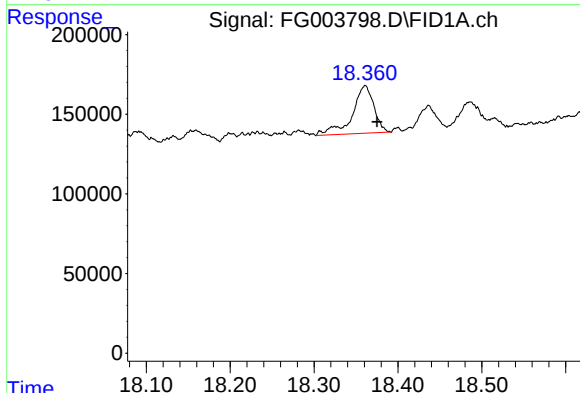


#14 N-DOTRIACONTANE

R.T.: 18.361 min
Delta R.T.: -0.014 min
Response: 534312
Conc: 4.08 ug/ml

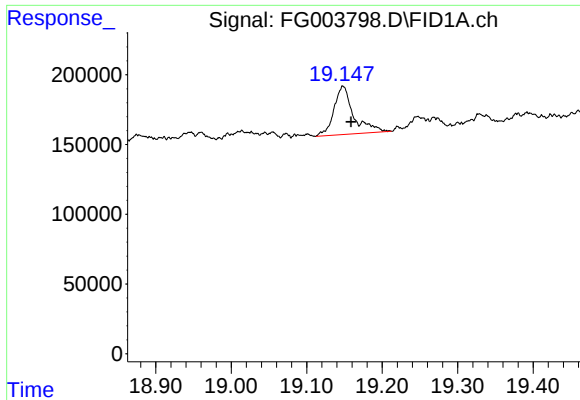


#15 N-TETRATRIACONTANE

R.T.: 19.148 min
Delta R.T.: -0.011 min
Response: 625462
Conc: 5.30 ug/ml

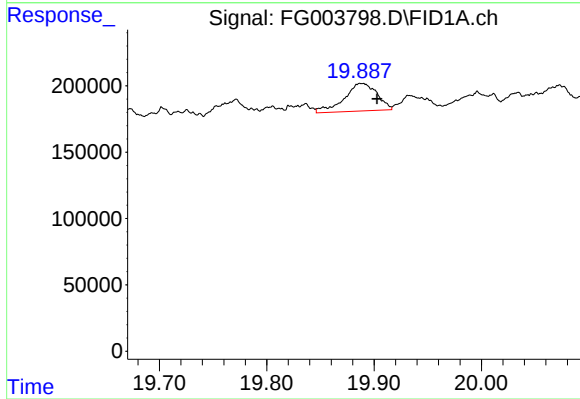

#16 N-HEXATRIACONTANE

R.T.: 19.888 min
Delta R.T.: -0.014 min
Response: 440242
Conc: 4.17 ug/ml

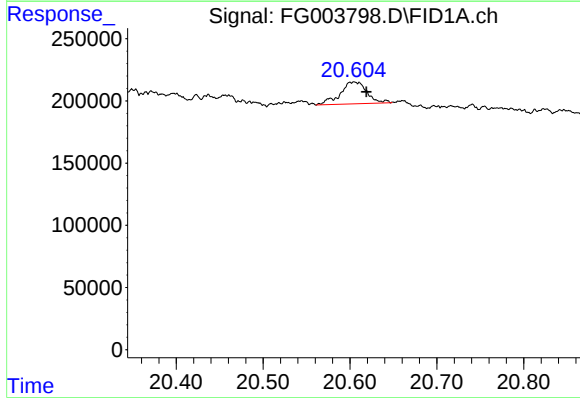

#17 N-OCTATRIACONTANE

R.T.: 20.610 min
Delta R.T.: -0.009 min
Response: 376772
Conc: 3.85 ug/ml