

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021320\
 Data File : FG006706.D
 Signal(s) : FID1A.ch
 Acq On : 13 Feb 2020 11:23
 Operator : DD\AJ
 Sample : L1491-04 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 00:42:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
 Quant Title :
 QLast Update : Tue Feb 11 13:28:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.615	167141	1.642 ug/ml
Target Compounds			
4) N-TETRADECANE	8.331	81764	0.834 ug/ml
7) N-EICOSANE	12.576	184690	1.645 ug/ml
10) N-TETRACOSANE	14.825	117378	1.010 ug/ml
12) N-OCTACOSANE	16.728	102814	0.873 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG021320\
Data File : FG006706.D
Signal(s) : FID1A.ch
Acq On : 13 Feb 2020 11:23
Operator : DD\AJ
Sample : L1491-04 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 00:42:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

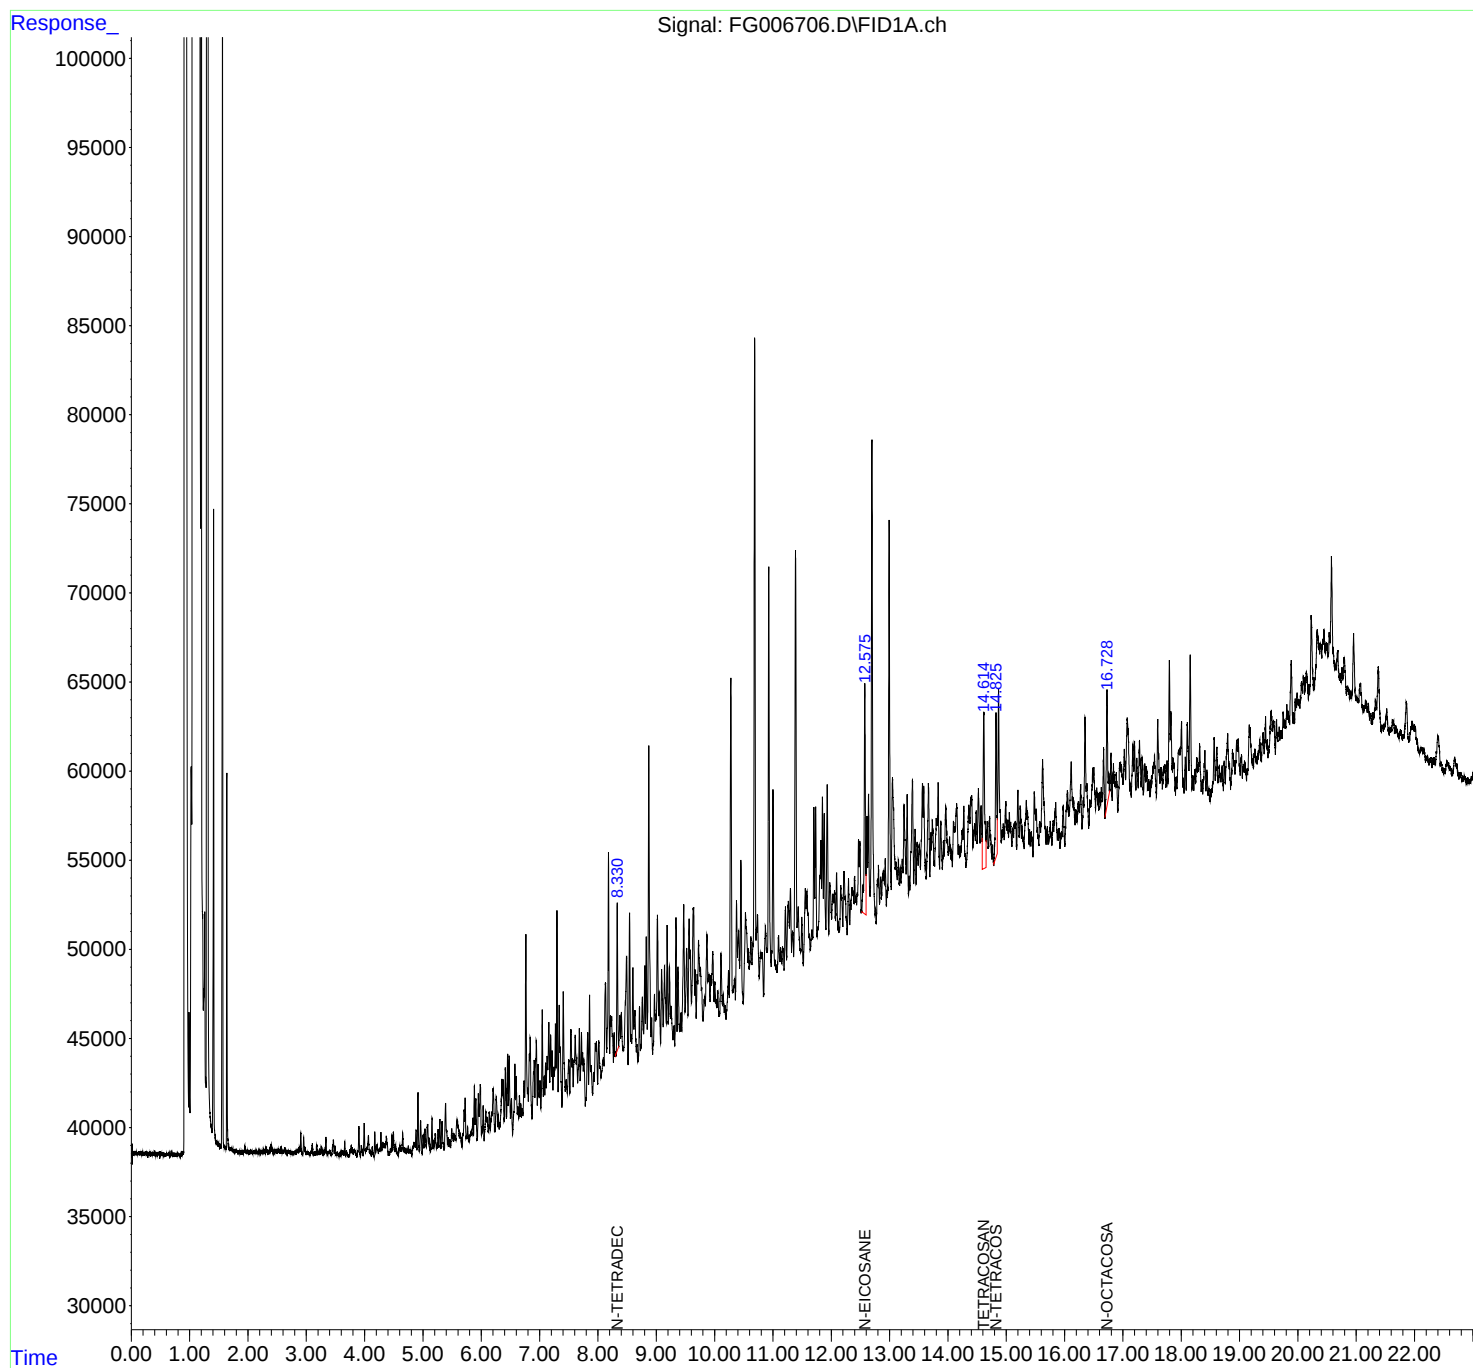


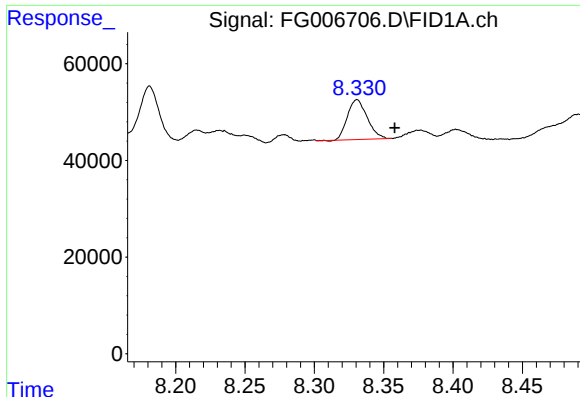

#4 N-TETRADECANE


R.T.: 8.331 min
Delta R.T.: -0.027 min
Response: 81764
Conc: 0.83 ug/ml

Instrument :
FID_G
ClientSampleId :

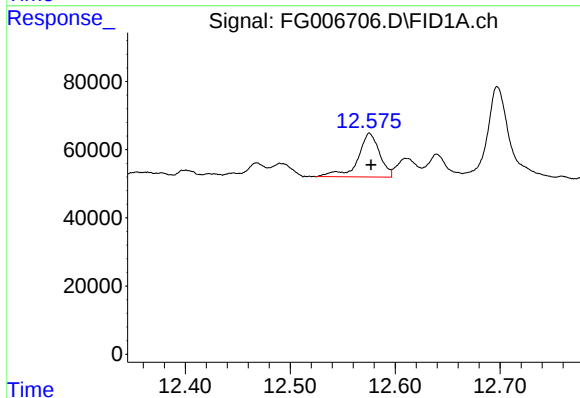


#7 N-EICOSANE

R.T.: 12.576 min
Delta R.T.: -0.001 min
Response: 184690
Conc: 1.65 ug/ml

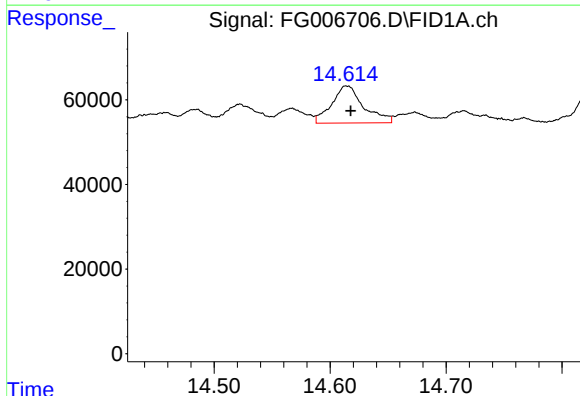


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.615 min
Delta R.T.: -0.003 min
Response: 167141
Conc: 1.64 ug/ml

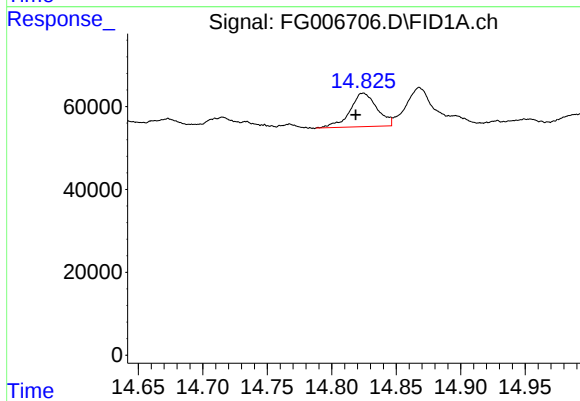

#10 N-TETRACOSANE

R.T.: 14.825 min
Delta R.T.: 0.006 min
Response: 117378
Conc: 1.01 ug/ml

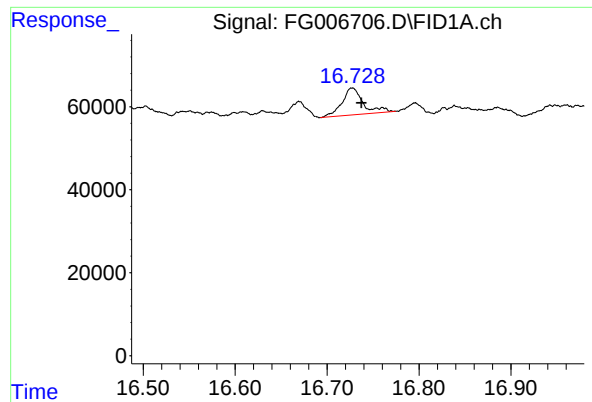

#12 N-OCTACOSANE

R.T.: 16.728 min
Delta R.T.: -0.010 min
Response: 102814
Conc: 0.87 ug/ml

Instrument :
FID_G
ClientSampleId :