

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG022120\
Data File : FG006727.D
Signal(s) : FID1A.ch
Acq On : 21 Feb 2020 14:37
Operator : DD\AJ
Sample : L1603-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:41:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	1565141	15.378 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.825	83287	0.717 ug/ml
12) N-OCTACOSANE	16.748	179534	1.525 ug/ml
13) N-TRIACONTANE	17.609	265259	2.210 ug/ml
14) N-DOTRIACONTANE	18.416	135567	1.220 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG022120\
Data File : FG006727.D
Signal(s) : FID1A.ch
Acq On : 21 Feb 2020 14:37
Operator : DD\AJ
Sample : L1603-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:41:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG021120.M
Quant Title :
QLast Update : Tue Feb 11 13:28:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

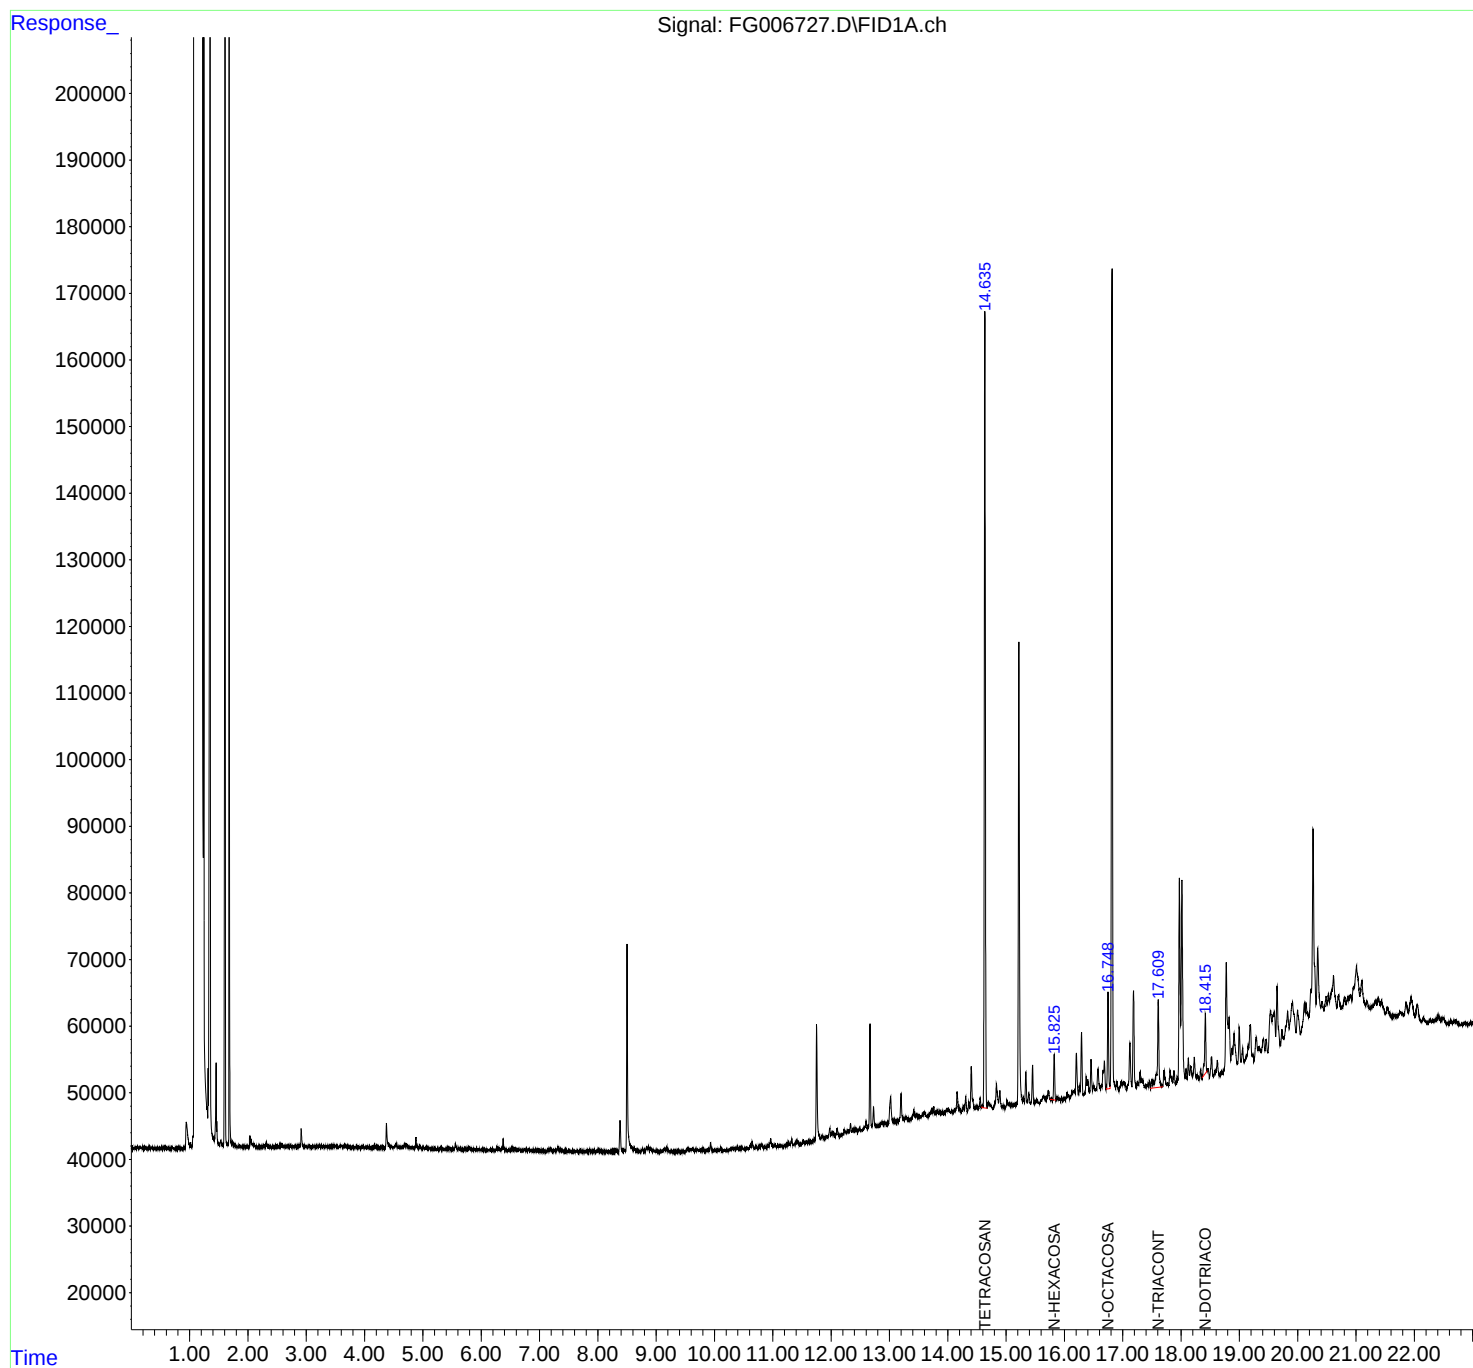


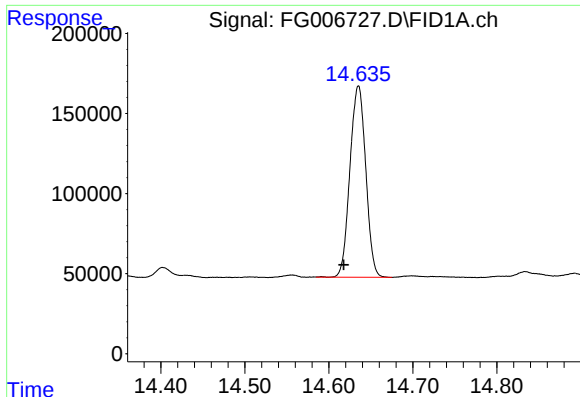

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.635 min
Delta R.T.: 0.017 min
Response: 1565141
Conc: 15.38 ug/ml

Instrument :
FID_G
ClientSampleId :

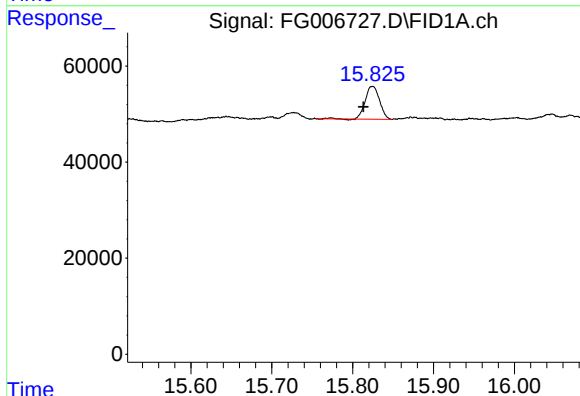


#11 N-HEXACOSANE

R.T.: 15.825 min
Delta R.T.: 0.011 min
Response: 83287
Conc: 0.72 ug/ml

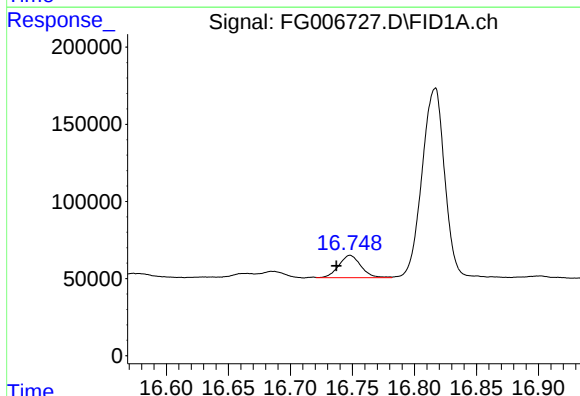


#12 N-OCTACOSANE

R.T.: 16.748 min
Delta R.T.: 0.011 min
Response: 179534
Conc: 1.52 ug/ml

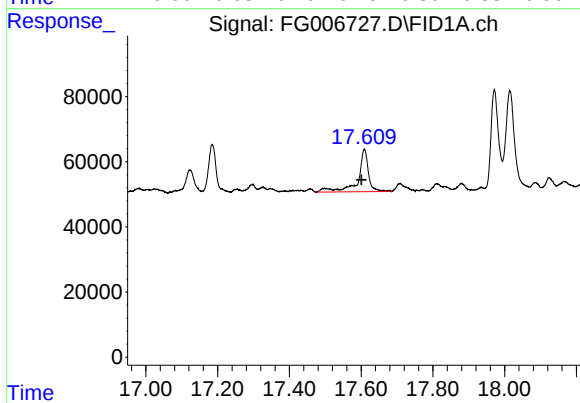

#13 N-TRIACONTANE

R.T.: 17.609 min
Delta R.T.: 0.008 min
Response: 265259
Conc: 2.21 ug/ml

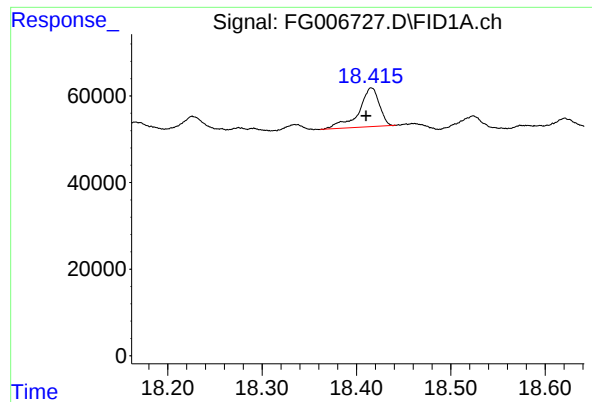

#14 N-DOTRIACONTANE

R.T.: 18.416 min
Delta R.T.: 0.005 min
Response: 135567
Conc: 1.22 ug/ml

Instrument :
FID_G
ClientSampleId :