

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG022323\
 Data File : FG011461.D
 Signal(s) : FID1A.ch
 Acq On : 23 Feb 2023 16:26
 Operator : YP\AJ
 Sample : 01627-03
 Misc : 1 PPM SOIL MDL
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 23 16:49:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:44:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.065	2259458	21.482 ug/ml
Target Compounds			
2) N-DECANE	4.590	142710	1.171 ug/ml
3) N-DODECANE	6.758	139693	1.130 ug/ml
4) N-TETRADECANE	8.589	118667	0.960 ug/ml
5) N-HEXADECANE	10.200	146535	1.161 ug/ml
6) N-OCTADECANE	11.647	148332	1.175 ug/ml
7) N-EICOSANE	12.960	148301	1.185 ug/ml
8) N-DOCOSANE	14.161	141177	1.177 ug/ml
10) N-TETRACOSANE	15.267	140657	1.192 ug/ml
11) N-HEXACOSANE	16.292	136836	1.202 ug/ml
12) N-OCTACOSANE	17.244	149135	1.359 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG022323\
Data File : FG011461.D
Signal(s) : FID1A.ch
Acq On : 23 Feb 2023 16:26
Operator : YP\AJ
Sample : 01627-03
Misc : 1 PPM SOIL MDL
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 23 16:49:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

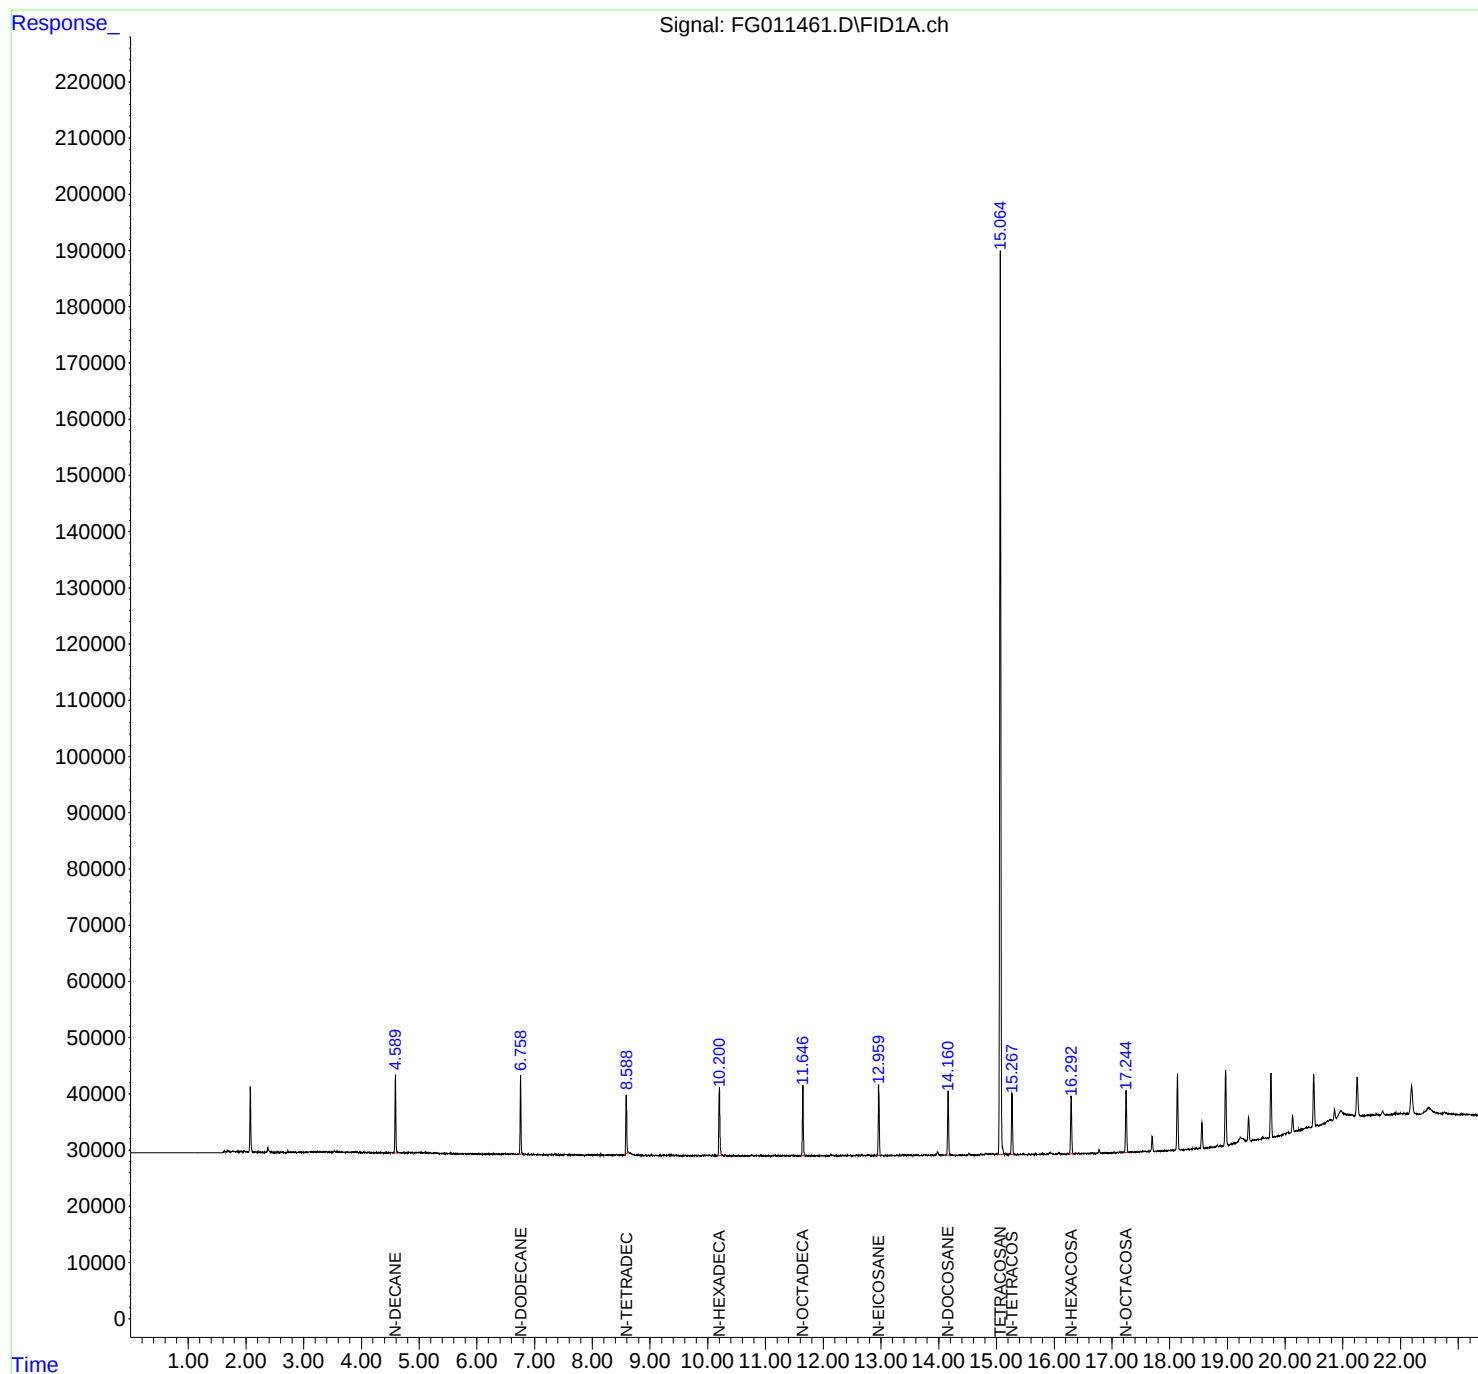

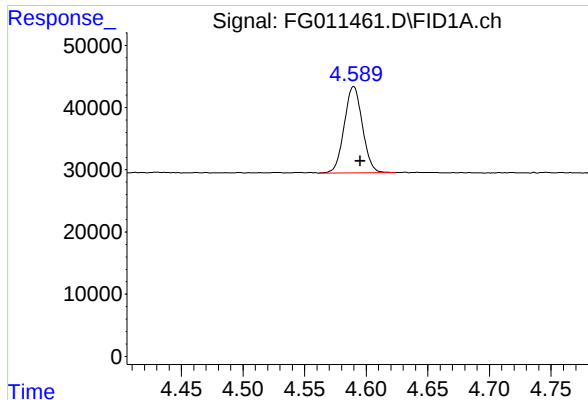


#2 N-DECANE

R.T.: 4.590 min
Delta R.T.: -0.005 min
Response: 142710
Conc: 1.17 ug/ml

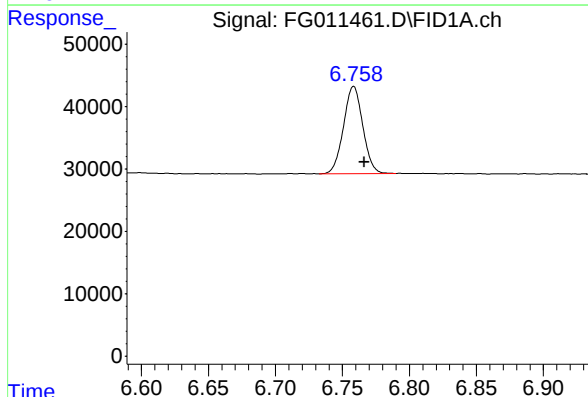


#3 N-DODECANE

R.T.: 6.758 min
Delta R.T.: -0.008 min
Response: 139693
Conc: 1.13 ug/ml

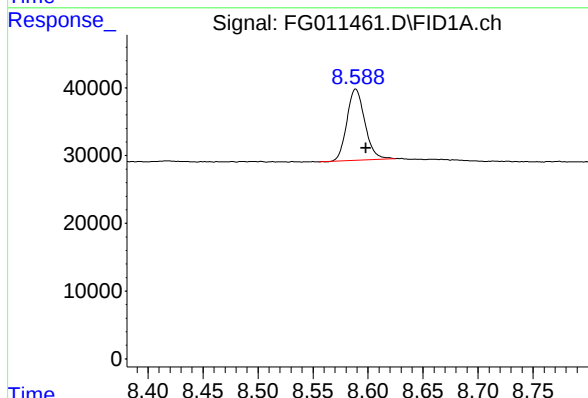


#4 N-TETRADECANE

R.T.: 8.589 min
Delta R.T.: -0.009 min
Response: 118667
Conc: 0.96 ug/ml

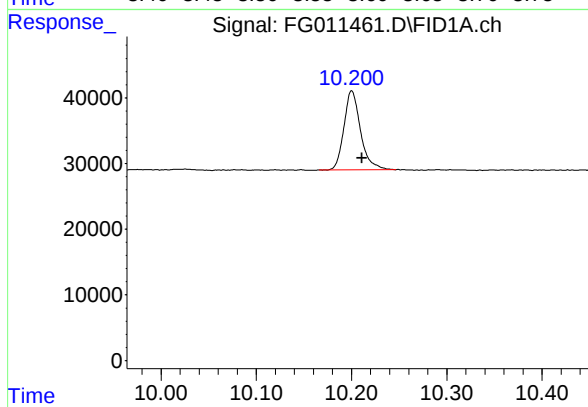


#5 N-HEXADECANE

R.T.: 10.200 min
Delta R.T.: -0.011 min
Response: 146535
Conc: 1.16 ug/ml

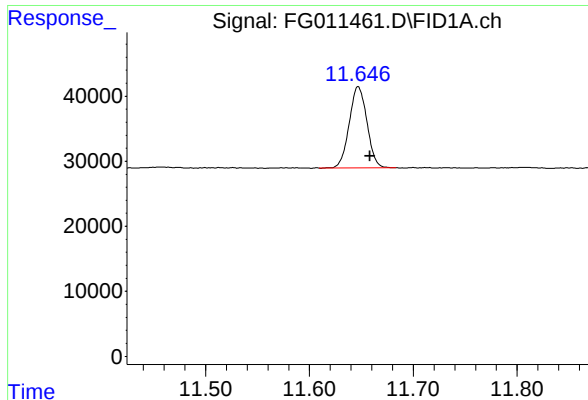


#6 N-OCTADECANE

R.T.: 11.647 min
Delta R.T.: -0.011 min
Response: 148332
Conc: 1.17 ug/ml

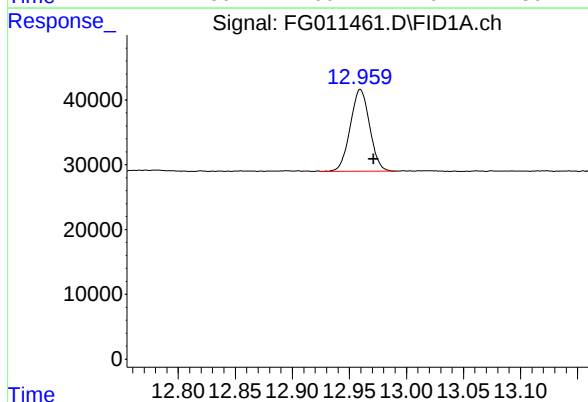


#7 N-EICOSANE

R.T.: 12.960 min
Delta R.T.: -0.012 min
Response: 148301
Conc: 1.18 ug/ml

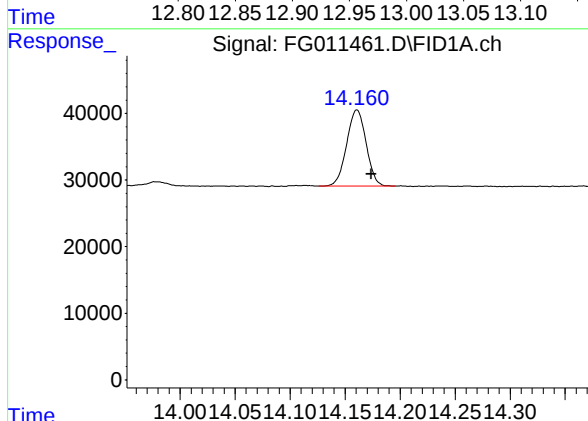


#8 N-DOCOSANE

R.T.: 14.161 min
Delta R.T.: -0.013 min
Response: 141177
Conc: 1.18 ug/ml

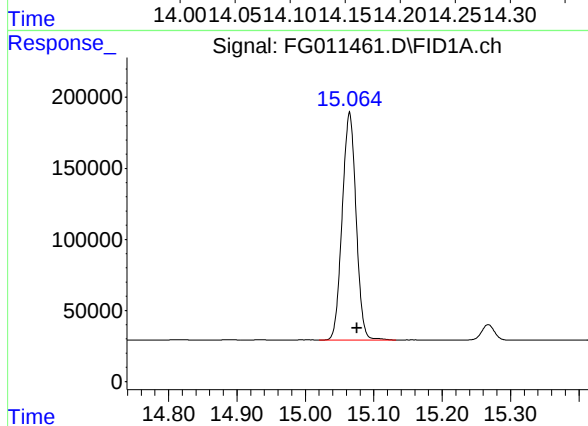


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.065 min
Delta R.T.: -0.011 min
Response: 2259458
Conc: 21.48 ug/ml

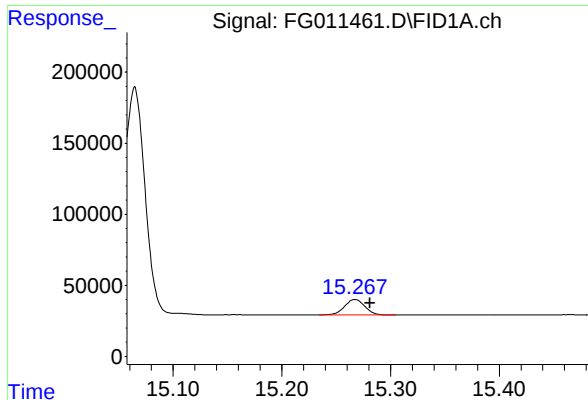


#10 N-TETRACOSANE

R.T.: 15.267 min
Delta R.T.: -0.014 min
Response: 140657
Conc: 1.19 ug/ml

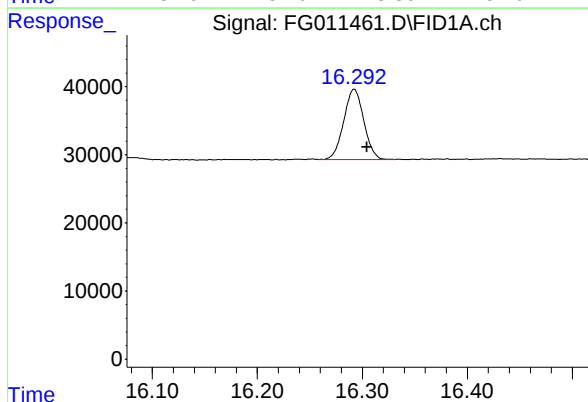

#11 N-HEXACOSANE

R.T.: 16.292 min
Delta R.T.: -0.012 min
Response: 136836
Conc: 1.20 ug/ml

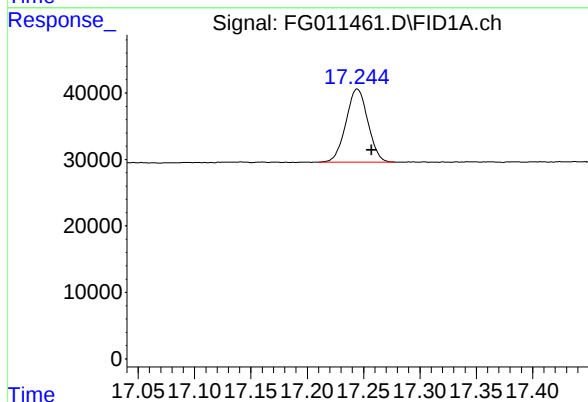

#12 N-OCTACOSANE

R.T.: 17.244 min
Delta R.T.: -0.013 min
Response: 149135
Conc: 1.36 ug/ml