

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG022525\  
Data File : FG015394.D  
Signal(s) : FID1A.ch  
Acq On : 25 Feb 2025 09:00  
Operator : YP\AJ  
Sample : PB166849BL  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 26 00:24:37 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG021025.M  
Quant Title :  
QLast Update : Mon Feb 10 11:26:50 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                          | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 15.037 | 1746132  | 16.094 ug/ml |
| Target Compounds            |                          |        |          |              |
| 14)                         | N-DOTRIACONTANE          | 18.942 | 29661    | 0.261 ug/ml  |
| 15)                         | N-TETRATRIACONTANE       | 19.725 | 21145    | 0.197 ug/ml  |
| 16)                         | N-HEXATRIACONTANE        | 20.467 | 23610    | 0.236 ug/ml  |
| 17)                         | N-OCTATRIACONTANE        | 21.214 | 41234    | 0.412 ug/ml  |
| -----                       |                          |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG022525\  
Data File : FG015394.D  
Signal(s) : FID1A.ch  
Acq On : 25 Feb 2025 09:00  
Operator : YP\AJ  
Sample : PB166849BL  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 26 00:24:37 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG021025.M  
Quant Title :  
QLast Update : Mon Feb 10 11:26:50 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

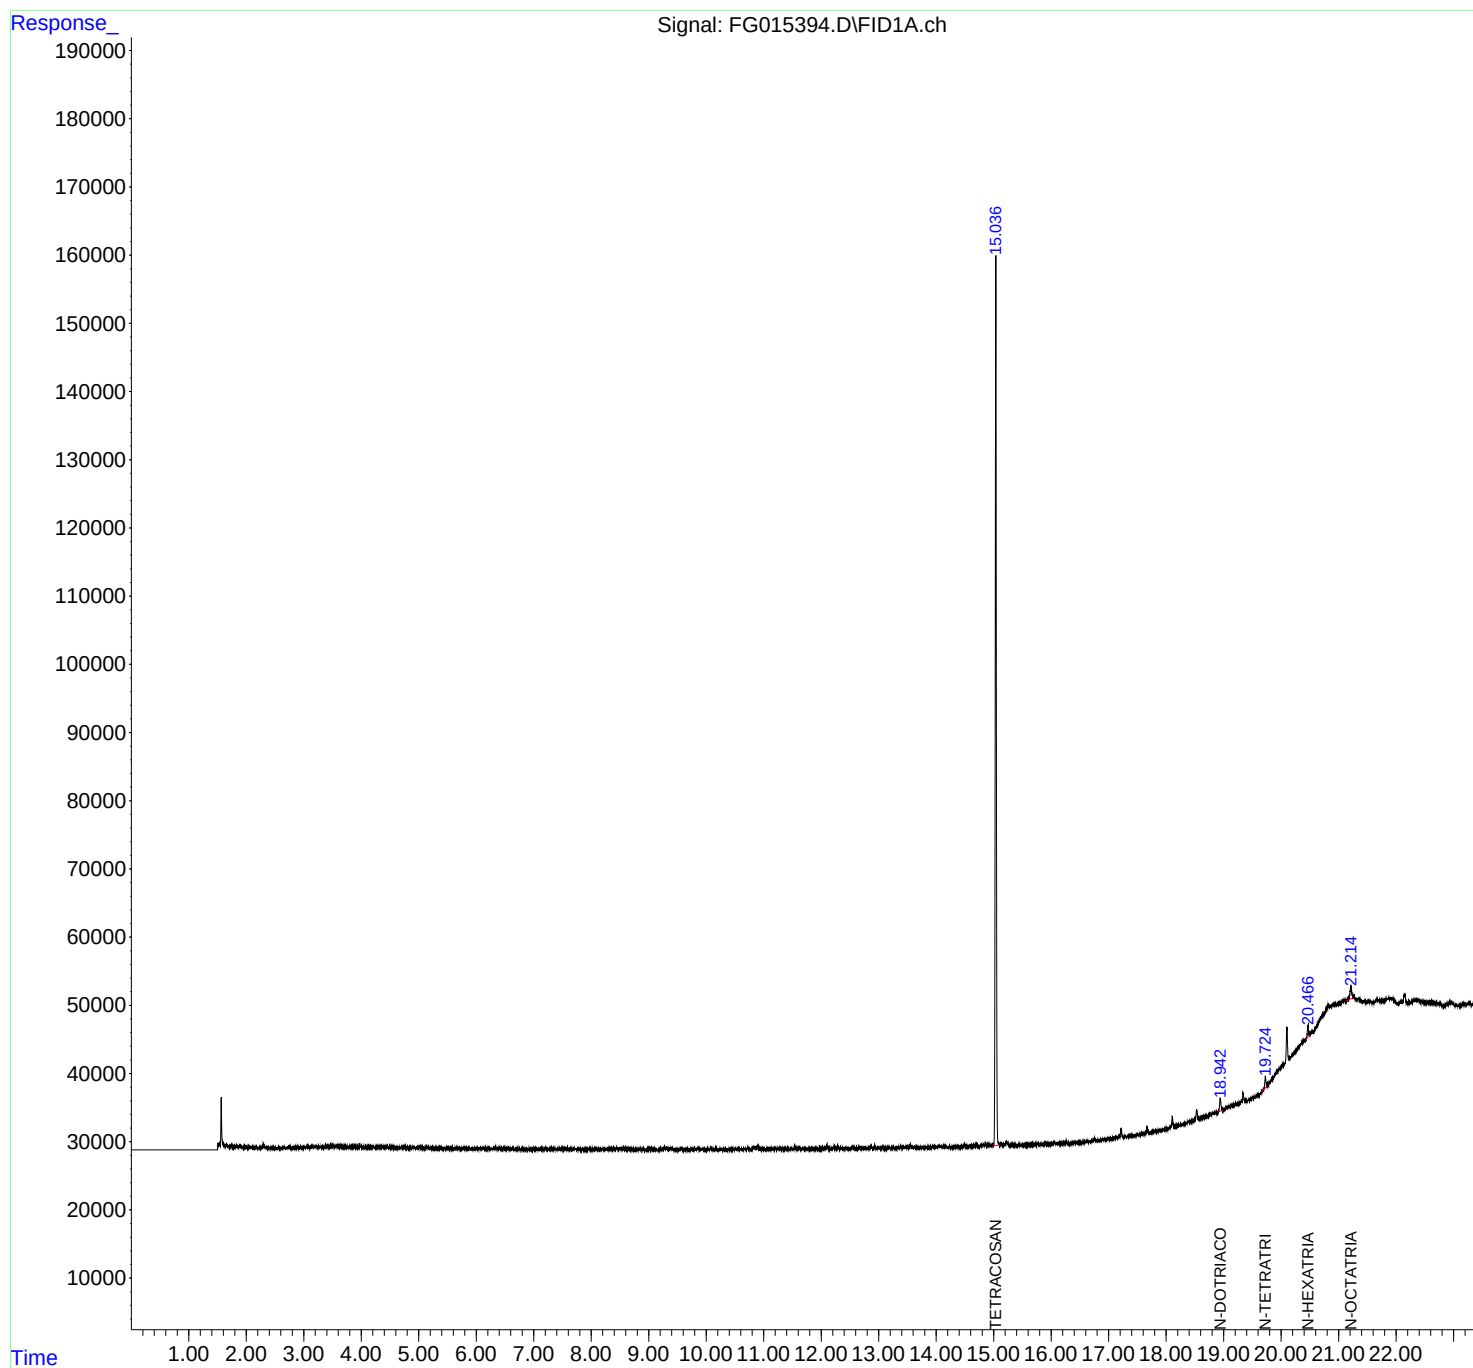


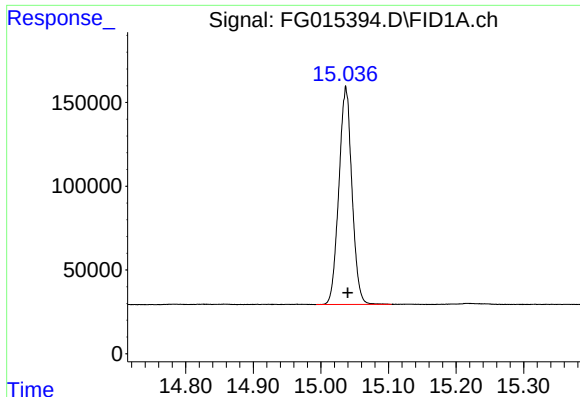

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.037 min  
Delta R.T.: -0.003 min  
Response: 1746132  
Conc: 16.09 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

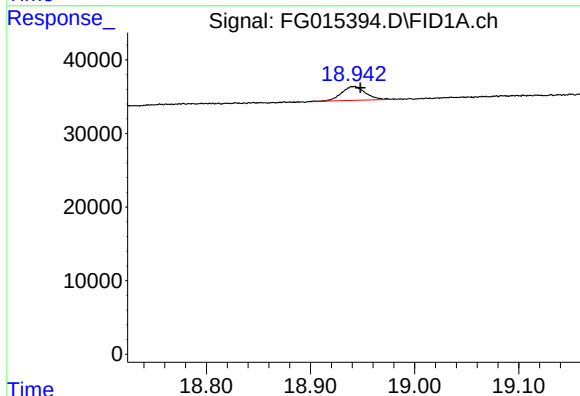


#14 N-DOTRIACONTANE

R.T.: 18.942 min  
Delta R.T.: -0.006 min  
Response: 29661  
Conc: 0.26 ug/ml

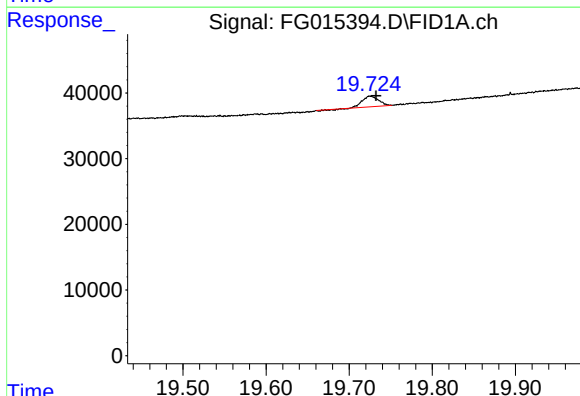


#15 N-TETRATRIACONTANE

R.T.: 19.725 min  
Delta R.T.: -0.008 min  
Response: 21145  
Conc: 0.20 ug/ml

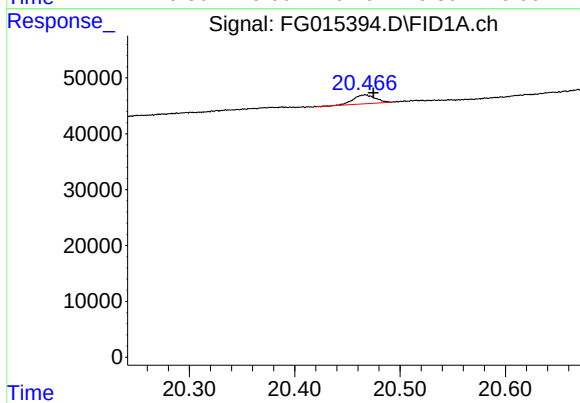

#16 N-HEXATRIACONTANE

R.T.: 20.467 min  
Delta R.T.: -0.008 min  
Response: 23610  
Conc: 0.24 ug/ml

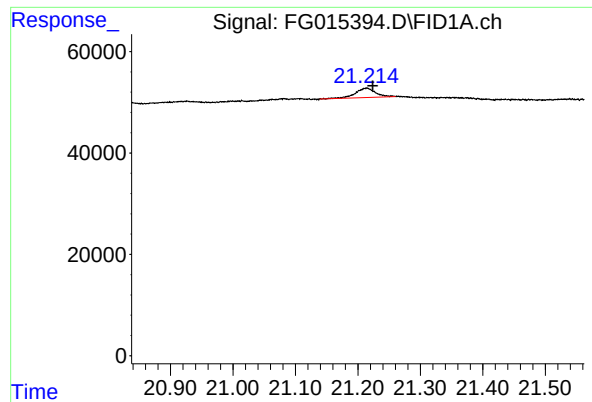

#17 N-OCTATRIACONTANE

R.T.: 21.214 min  
Delta R.T.: -0.010 min  
Response: 41234  
Conc: 0.41 ug/ml

Instrument :

FID\_G

ClientSampleId :