

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG022619\
 Data File : FG003954.D
 Signal(s) : FID1A.ch
 Acq On : 26 Feb 2019 11:51
 Operator : AJ\SJ
 Sample : K1348-05 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 27 00:33:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
 Quant Title :
 QLast Update : Wed Feb 06 08:50:01 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.458	797885	5.899 ug/ml
Target Compounds				
7)	N-EICOSANE	12.400	1754853	11.205 ug/ml
8)	N-DOCOSANE	13.562	230919	1.493 ug/ml
10)	N-TETRACOSANE	14.622f	517723	3.436 ug/ml
11)	N-HEXACOSANE	15.684	194260	1.321 ug/ml
12)	N-OCTACOSANE	16.635	444755	3.087 ug/ml
13)	N-TRIACONTANE	17.526	456383	3.225 ug/ml
14)	N-DOTRIACONTANE	18.363	299204	2.285 ug/ml
15)	N-TETRATRIACONTANE	19.149	291654	2.473 ug/ml
16)	N-HEXATRIACONTANE	19.892	449439	4.258 ug/ml
17)	N-OCTATRIACONTANE	20.613	453118	4.635 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG022619\
Data File : FG003954.D
Signal(s) : FID1A.ch
Acq On : 26 Feb 2019 11:51
Operator : AJ\SJ
Sample : K1348-05 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 27 00:33:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG020519.M
Quant Title :
QLast Update : Wed Feb 06 08:50:01 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

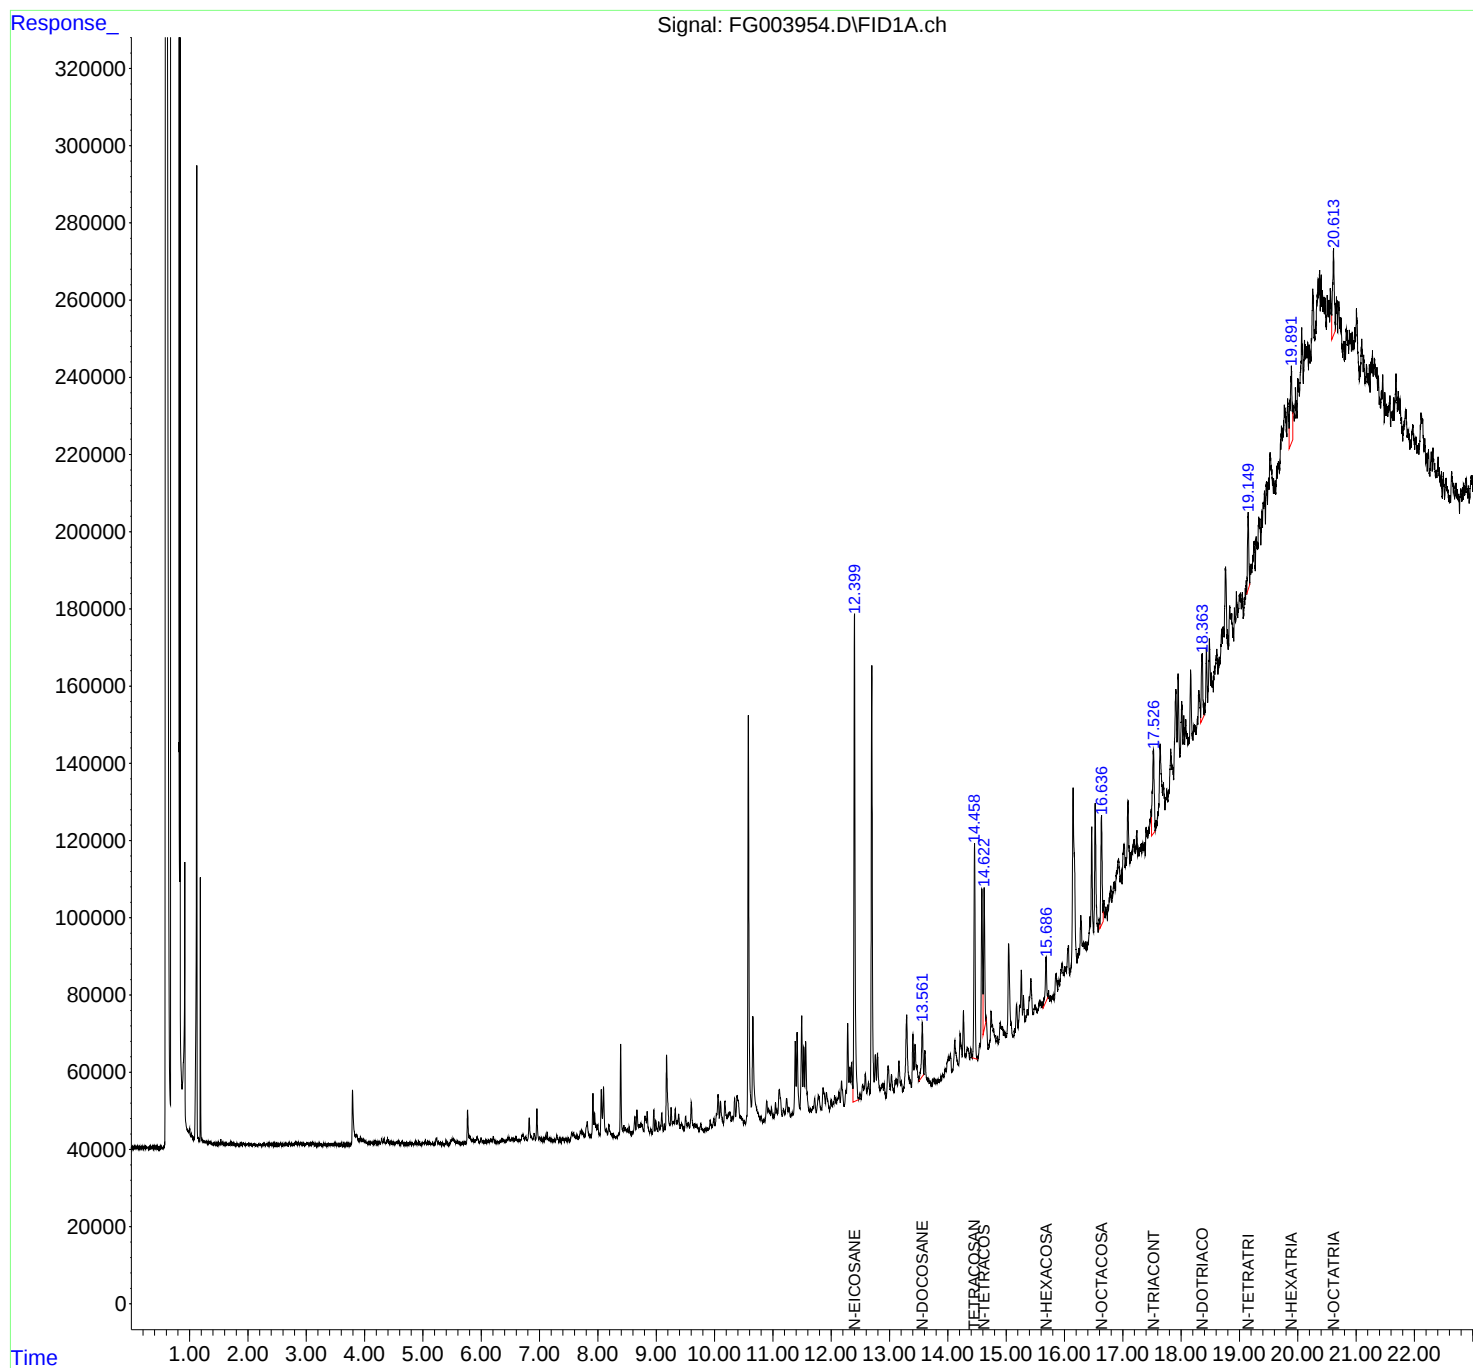

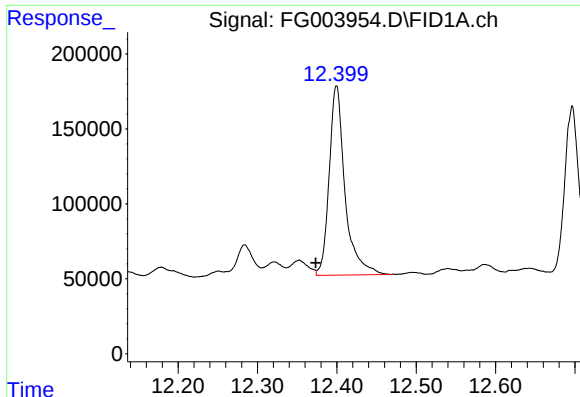


#7 N-EICOSANE

R.T.: 12.400 min
Delta R.T.: 0.026 min
Response: 1754853
Conc: 11.20 ug/ml

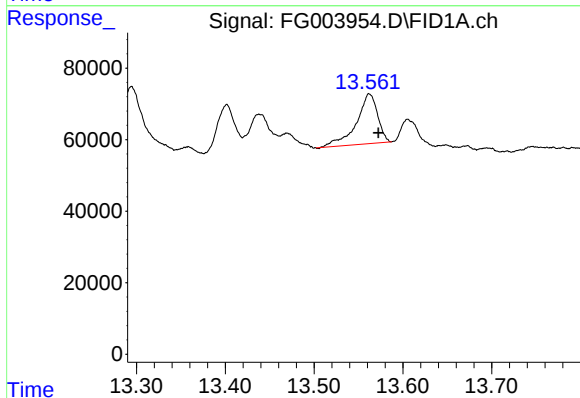


#8 N-DOCOSANE

R.T.: 13.562 min
Delta R.T.: -0.010 min
Response: 230919
Conc: 1.49 ug/ml

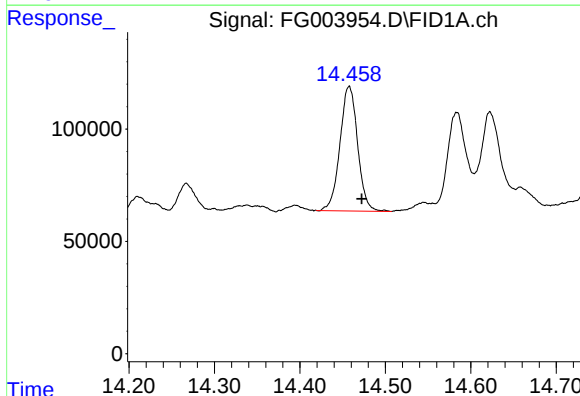


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.015 min
Response: 797885
Conc: 5.90 ug/ml

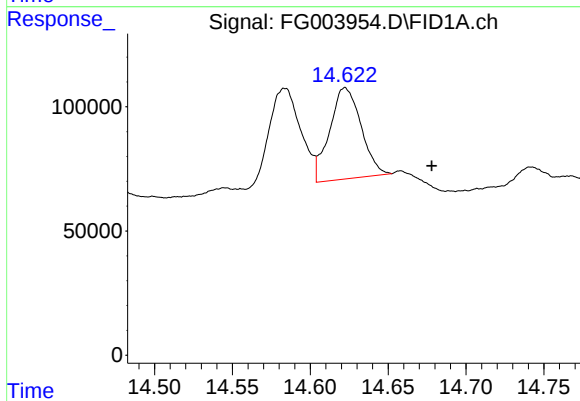


#10 N-TETRACOSANE

R.T.: 14.622 min
Delta R.T.: -0.056 min
Response: 517723
Conc: 3.44 ug/ml

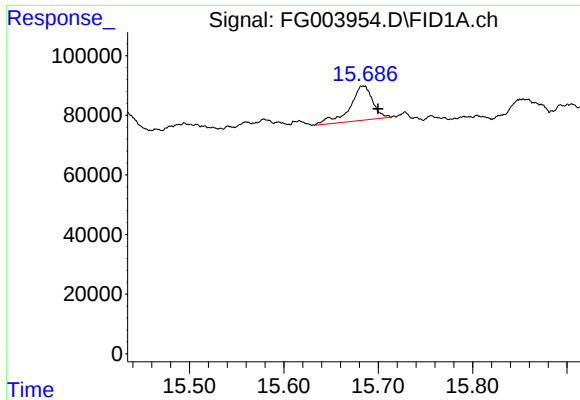


#11 N-HEXACOSANE

R.T.: 15.684 min
Delta R.T.: -0.016 min
Response: 194260
Conc: 1.32 ug/ml

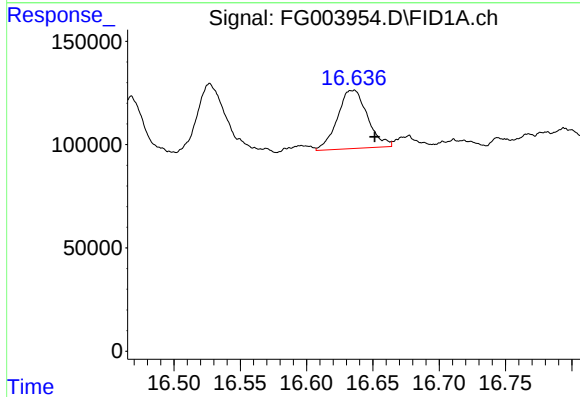


#12 N-OCTACOSANE

R.T.: 16.635 min
Delta R.T.: -0.016 min
Response: 444755
Conc: 3.09 ug/ml

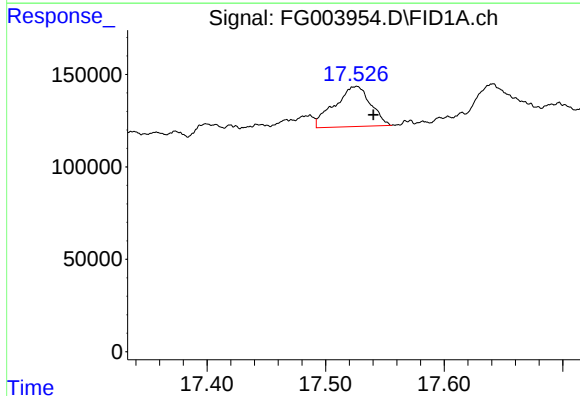


#13 N-TRIACONTANE

R.T.: 17.526 min
Delta R.T.: -0.015 min
Response: 456383
Conc: 3.22 ug/ml

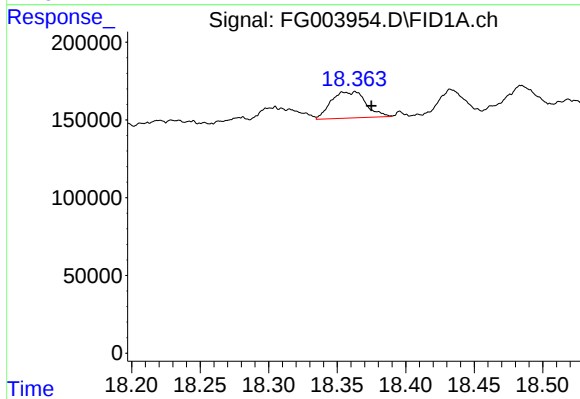

#14 N-DOTRIACONTANE

R.T.: 18.363 min
Delta R.T.: -0.011 min
Response: 299204
Conc: 2.28 ug/ml

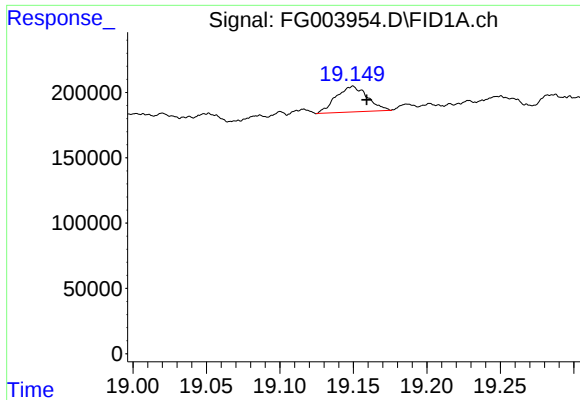


#15 N-TETRATRIACONTANE

R.T.: 19.149 min

Delta R.T.: -0.010 min

Response: 291654

Conc: 2.47 ug/ml

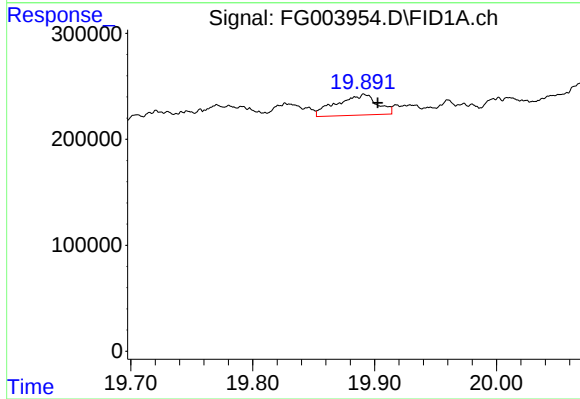


#16 N-HEXATRIACONTANE

R.T.: 19.892 min

Delta R.T.: -0.011 min

Response: 449439

Conc: 4.26 ug/ml

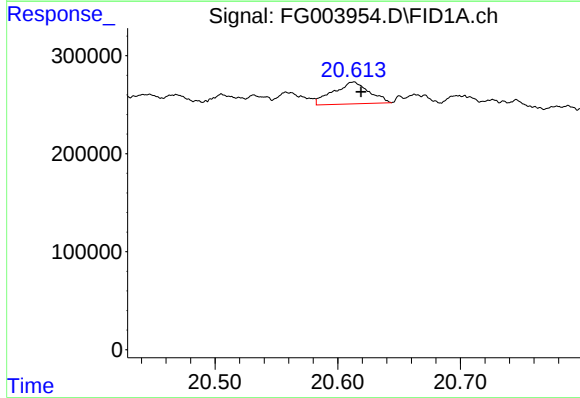

#17 N-OCTATRIACONTANE

R.T.: 20.613 min

Delta R.T.: -0.006 min

Response: 453118

Conc: 4.63 ug/ml