

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030323\
 Data File : FG011522.D
 Signal(s) : FID1A.ch
 Acq On : 03 Mar 2023 23:49
 Operator : YP\AJ
 Sample : 01767-15 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 00:57:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:44:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.063	172981	1.645 ug/ml
Target Compounds			
7) N-EICOSANE	13.023f	106667	0.852 ug/ml
10) N-TETRACOSANE	15.247	63760	0.540 ug/ml
14) N-DOTRIACONTANE	18.970	53139	0.527 ug/ml
15) N-TETRATRIACONTANE	19.755	19050	0.202 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030323\
Data File : FG011522.D
Signal(s) : FID1A.ch
Acq On : 03 Mar 2023 23:49
Operator : YP\AJ
Sample : 01767-15 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 00:57:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

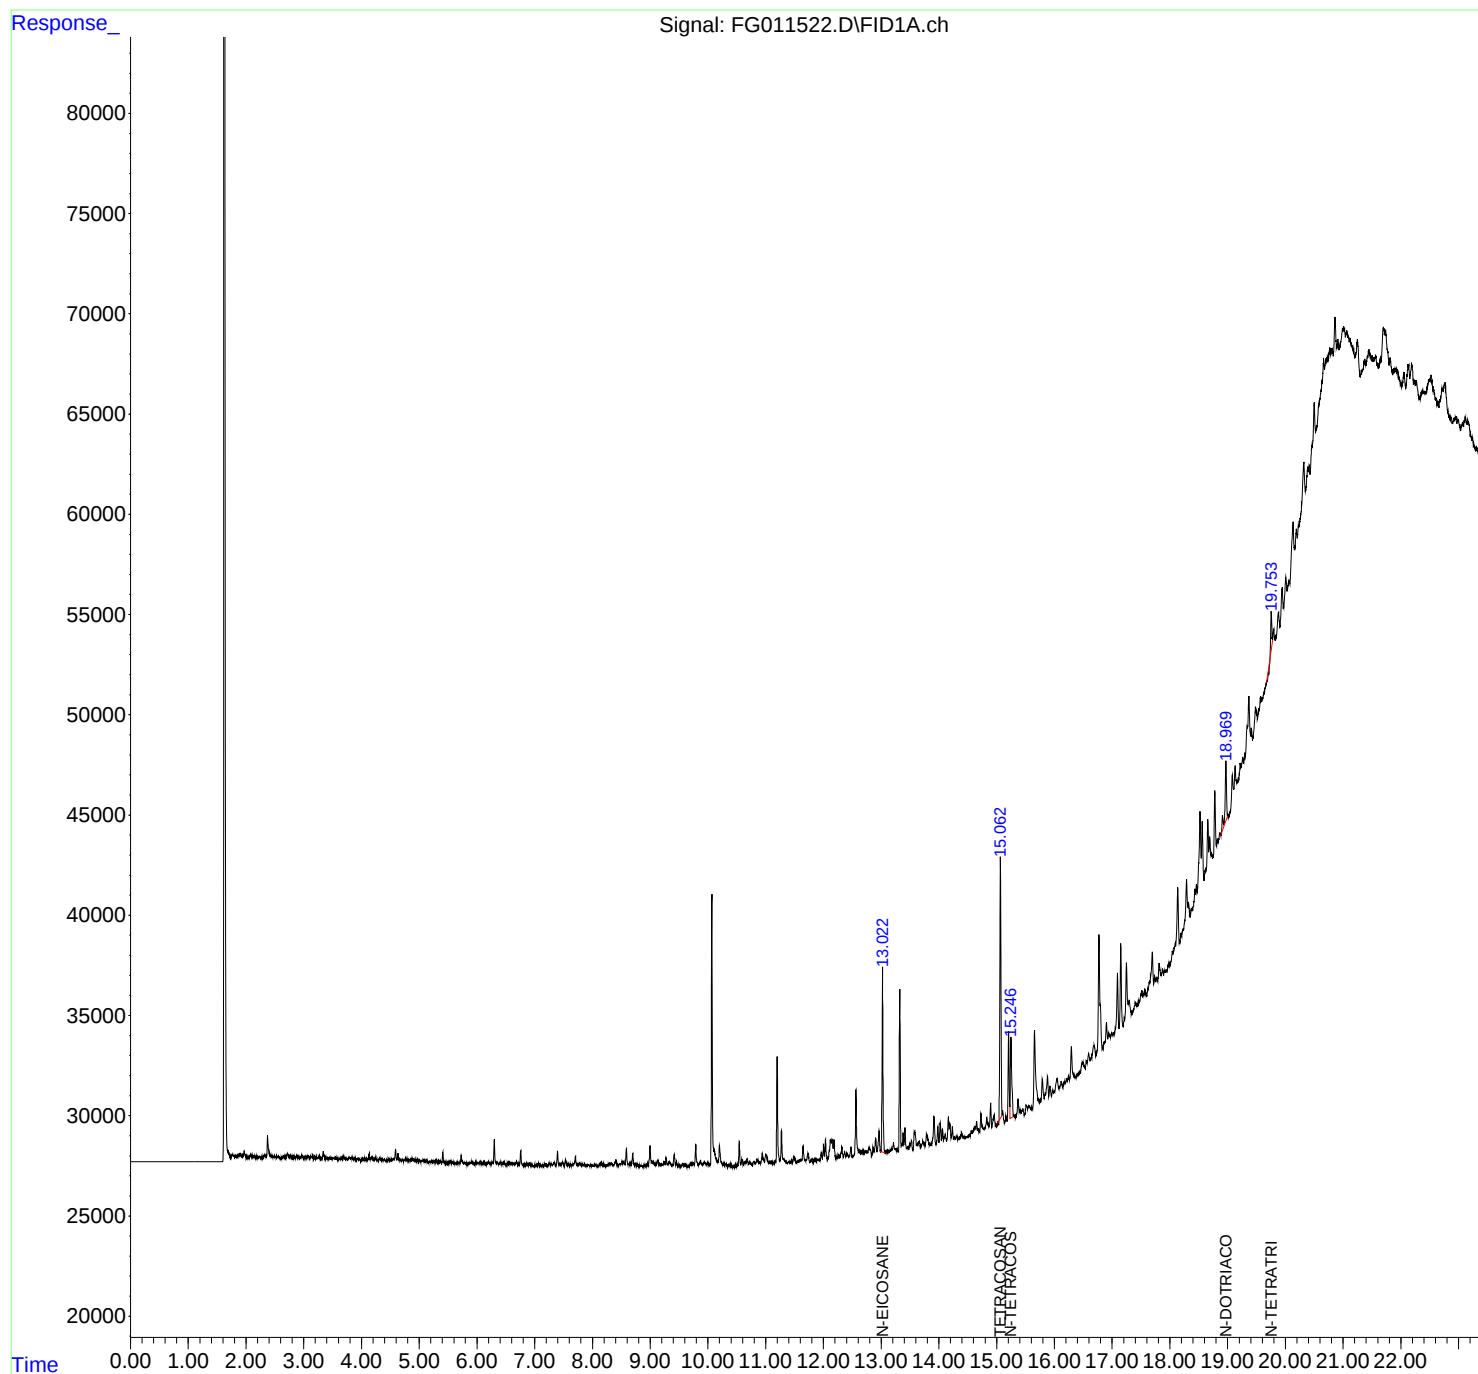

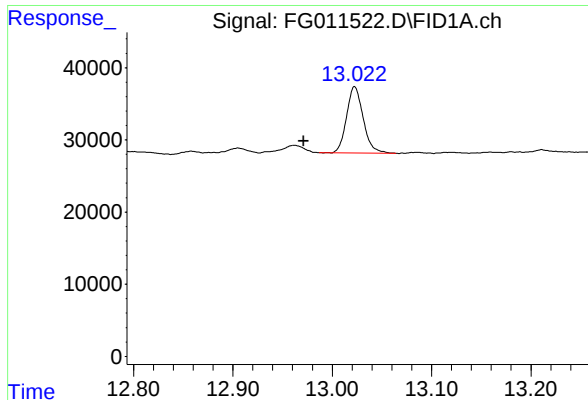


#7 N-EICOSANE

R.T.: 13.023 min
Delta R.T.: 0.051 min
Response: 106667
Conc: 0.85 ug/ml

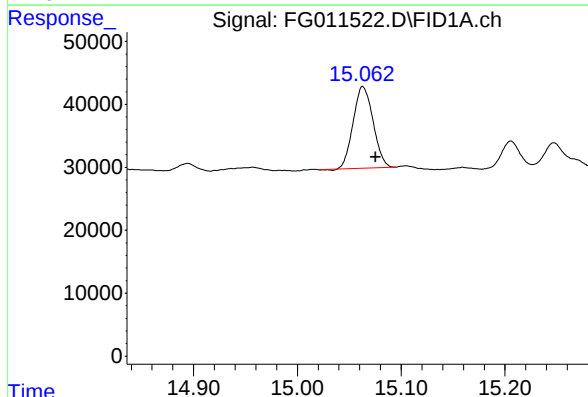


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.063 min
Delta R.T.: -0.012 min
Response: 172981
Conc: 1.64 ug/ml

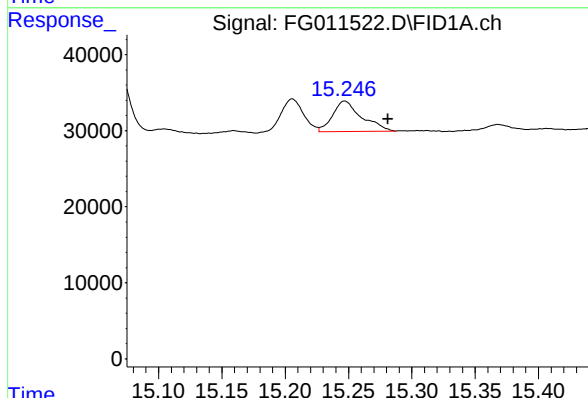


#10 N-TETRACOSANE

R.T.: 15.247 min
Delta R.T.: -0.034 min
Response: 63760
Conc: 0.54 ug/ml

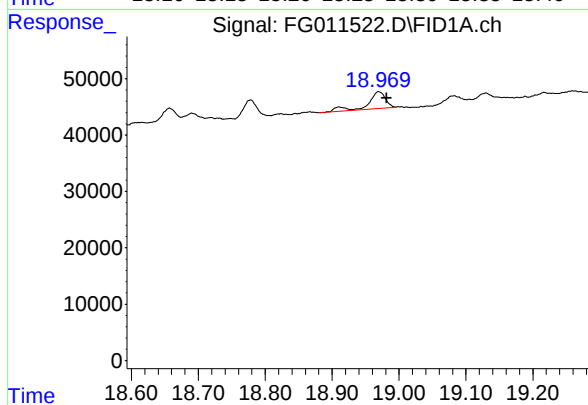

#14 N-DOTRIACONTANE

R.T.: 18.970 min
Delta R.T.: -0.012 min
Response: 53139
Conc: 0.53 ug/ml

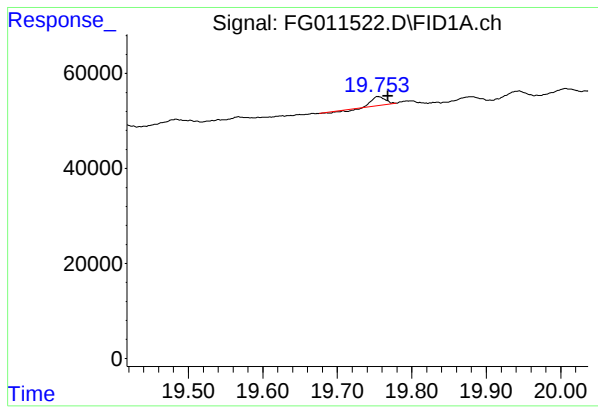

#15 N-TETRATRIACONTANE

R.T.: 19.755 min
Delta R.T.: -0.013 min
Response: 19050
Conc: 0.20 ug/ml