

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030425\
Data File : FG015442.D
Signal(s) : FID1A.ch
Acq On : 04 Mar 2025 19:14
Operator : YP\AJ
Sample : Q1474-01 20X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-03-02282025

Integration File: autoint1.e
Quant Time: Mar 05 01:41:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030325.M
Quant Title :
QLast Update : Mon Mar 03 14:06:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.043	96269	0.884 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030425\
Data File : FG015442.D
Signal(s) : FID1A.ch
Acq On : 04 Mar 2025 19:14
Operator : YP\AJ
Sample : Q1474-01 20X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-03-02282025

Integration File: autoint1.e
Quant Time: Mar 05 01:41:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030325.M
Quant Title :
QLast Update : Mon Mar 03 14:06:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

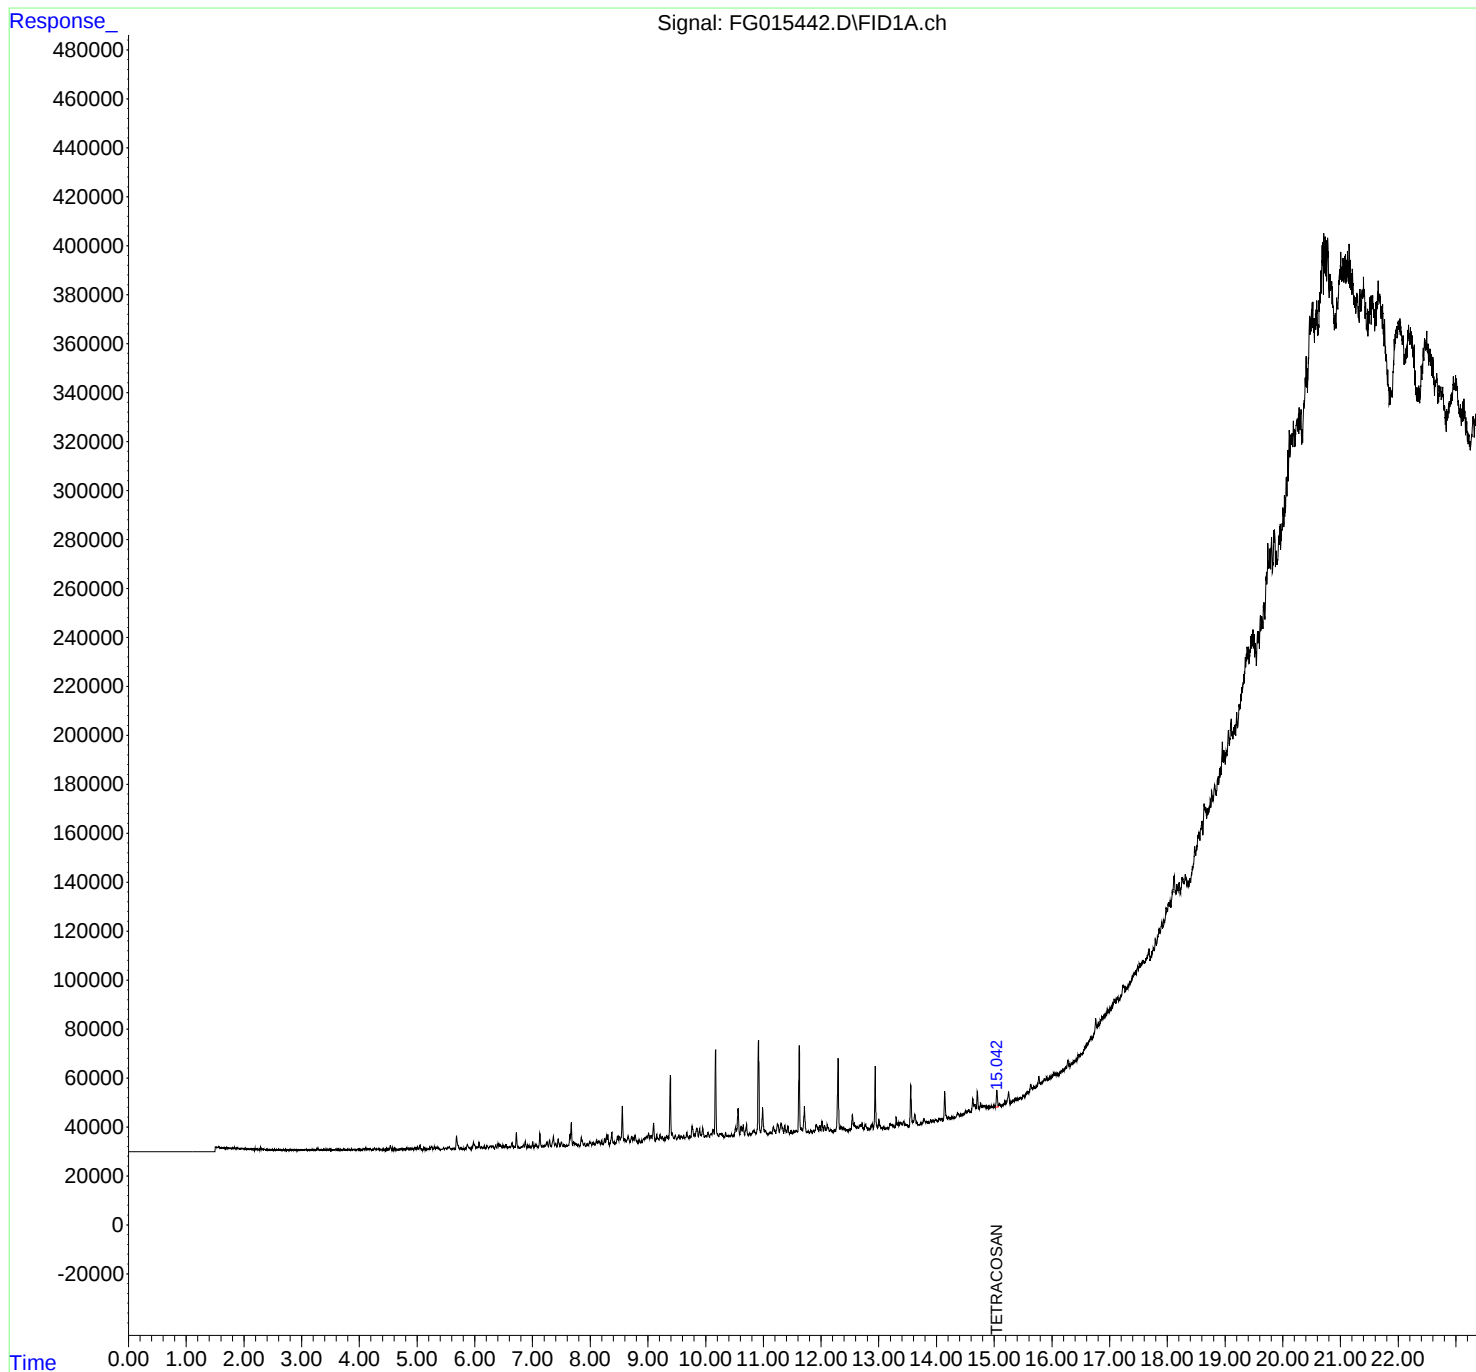

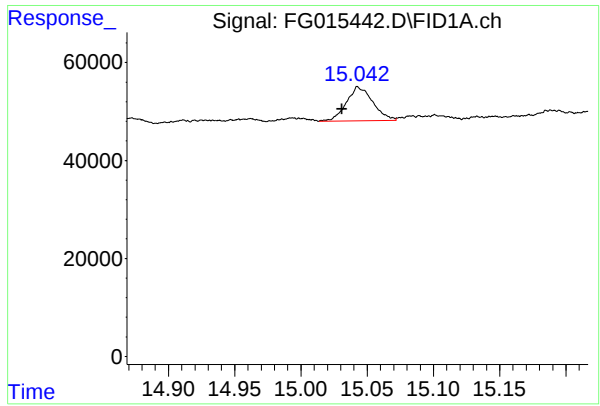

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.043 min
Delta R.T.: 0.012 min
Response: 96269
Conc: 0.88 ug/ml

Instrument :
FID_G
ClientSampleId :
BU-03-02282025