

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030519\
 Data File : FG004047.D
 Signal(s) : FID1A.ch
 Acq On : 05 Mar 2019 20:24
 Operator : AJ\SJ
 Sample : K1727-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 06 00:38:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.437	2202841	17.522 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.350	340440	2.691 ug/ml
16) N-HEXATRIACONTANE	19.906	683393	6.173 ug/ml
18) N-TETRACONTANE	21.446	881152	8.308 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030519\
Data File : FG004047.D
Signal(s) : FID1A.ch
Acq On : 05 Mar 2019 20:24
Operator : AJ\SJ
Sample : K1727-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 00:38:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

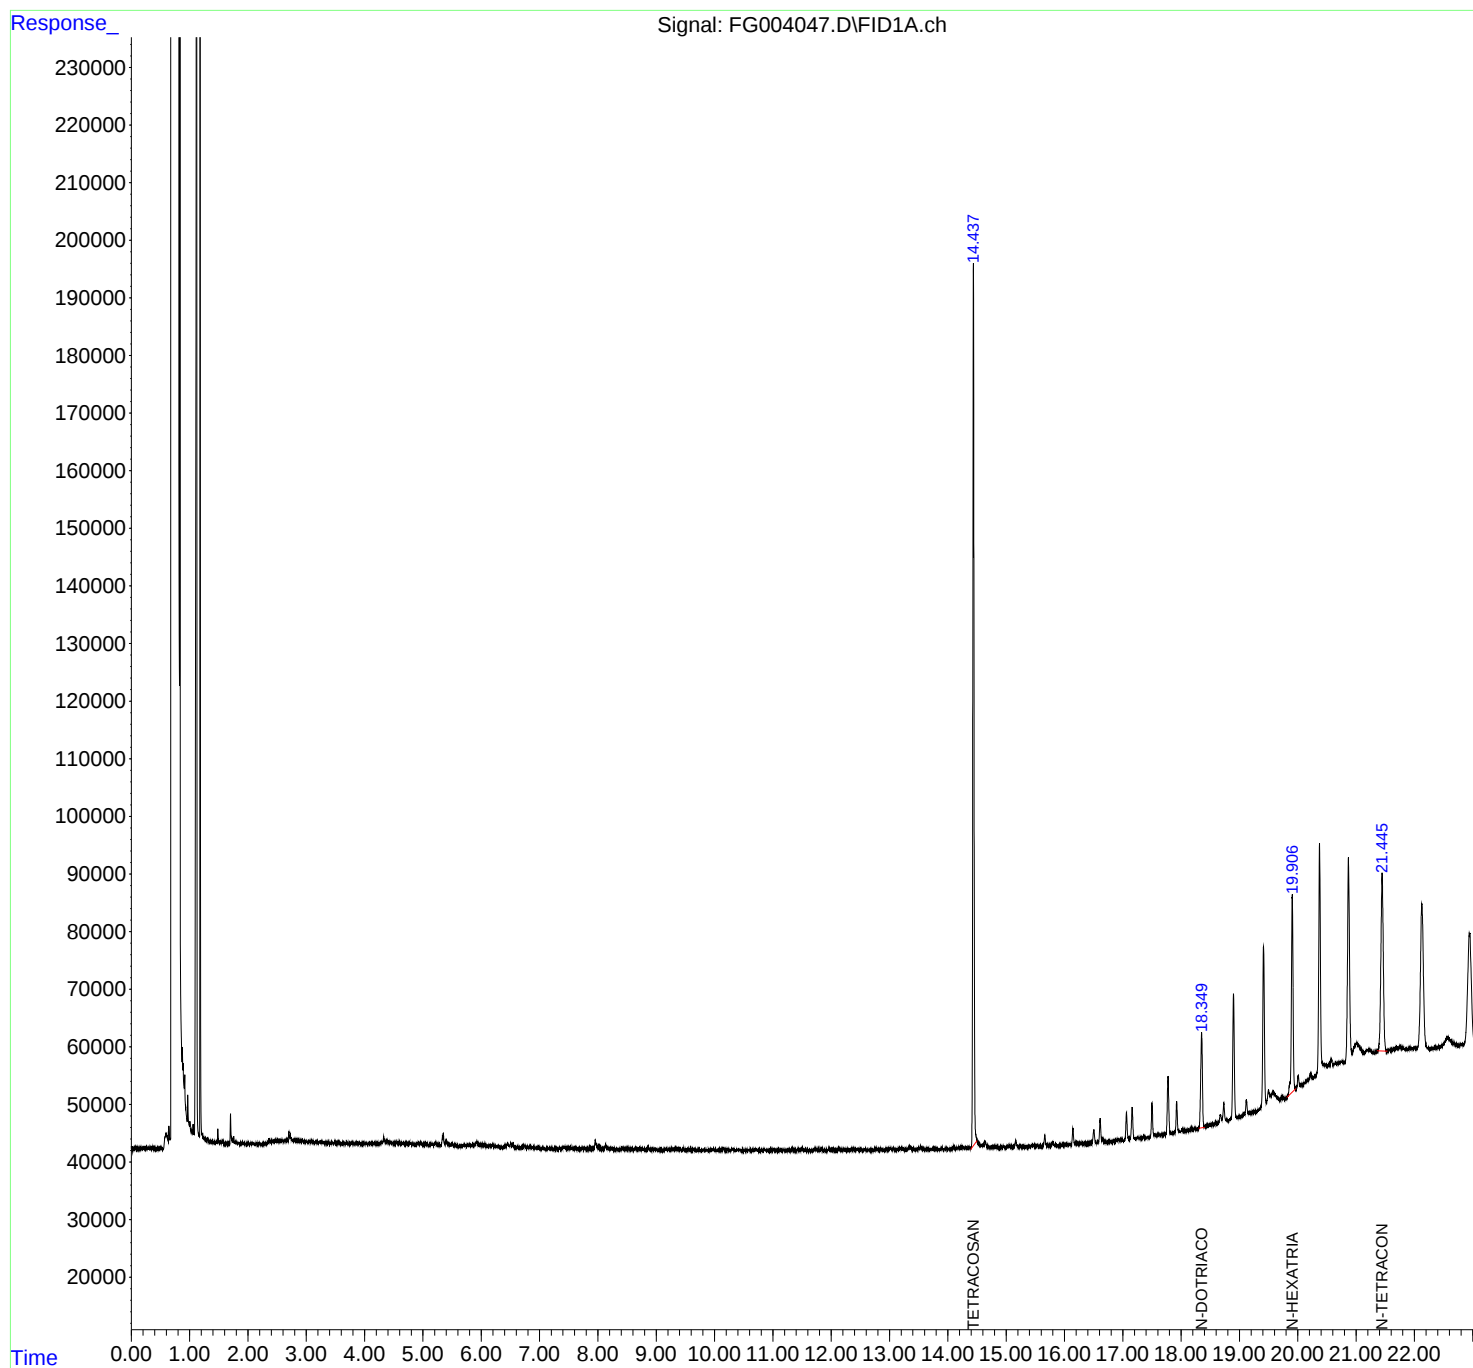


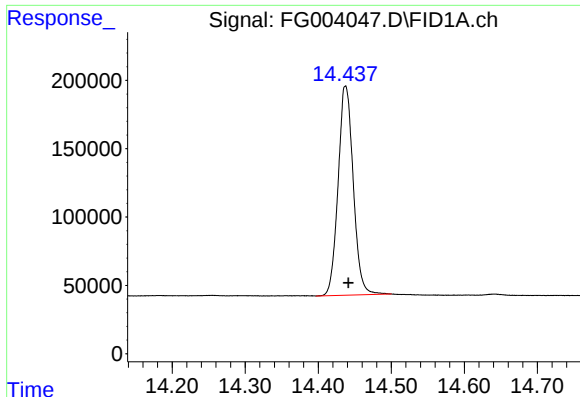

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.437 min
Delta R.T.: -0.004 min
Response: 2202841
Conc: 17.52 ug/ml

Instrument :
FID_G
ClientSampleId :

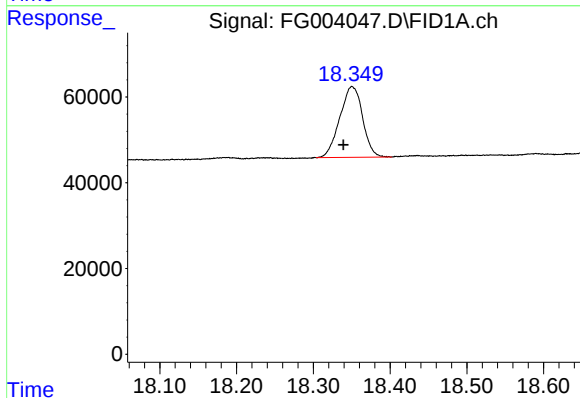


#14 N-DOTRIACONTANE

R.T.: 18.350 min
Delta R.T.: 0.011 min
Response: 340440
Conc: 2.69 ug/ml

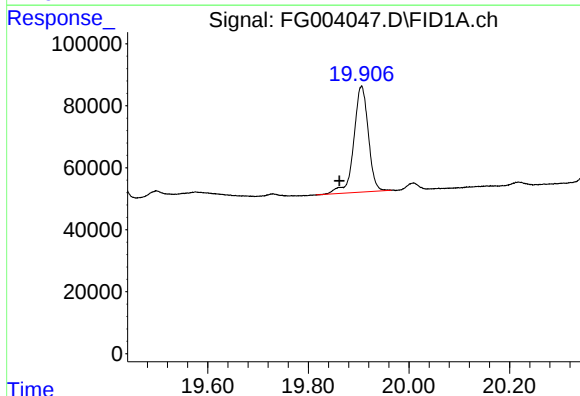

#16 N-HEXATRIACONTANE

R.T.: 19.906 min
Delta R.T.: 0.044 min
Response: 683393
Conc: 6.17 ug/ml

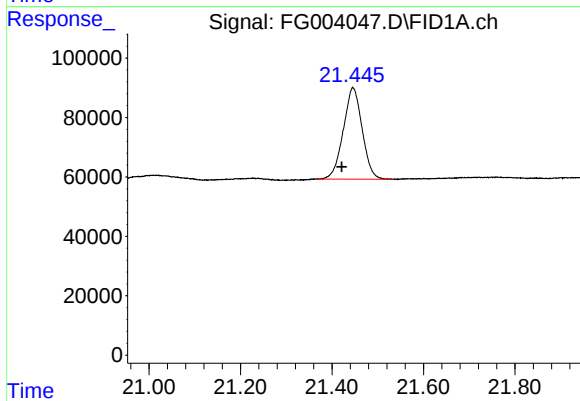

#18 N-TETRACONTANE

R.T.: 21.446 min
Delta R.T.: 0.024 min
Response: 881152
Conc: 8.31 ug/ml