

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030521\
 Data File : FG007636.D
 Signal(s) : FID1A.ch
 Acq On : 05 Mar 2021 17:46
 Operator : DD\AJ
 Sample : M1576-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 05 23:32:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
 Quant Title :
 QLast Update : Fri Mar 05 08:57:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	2510085	18.825 ug/ml
Target Compounds			
4) N-TETRADECANE	7.958	86124	0.534 ug/ml
14) N-DOTRIACONTANE	18.356	195313	1.523 ug/ml
15) N-TETRATRIACONTANE	19.152	51220	0.426 ug/ml
16) N-HEXATRIACONTANE	19.907	110359	0.969 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030521\
Data File : FG007636.D
Signal(s) : FID1A.ch
Acq On : 05 Mar 2021 17:46
Operator : DD\AJ
Sample : M1576-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 23:32:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

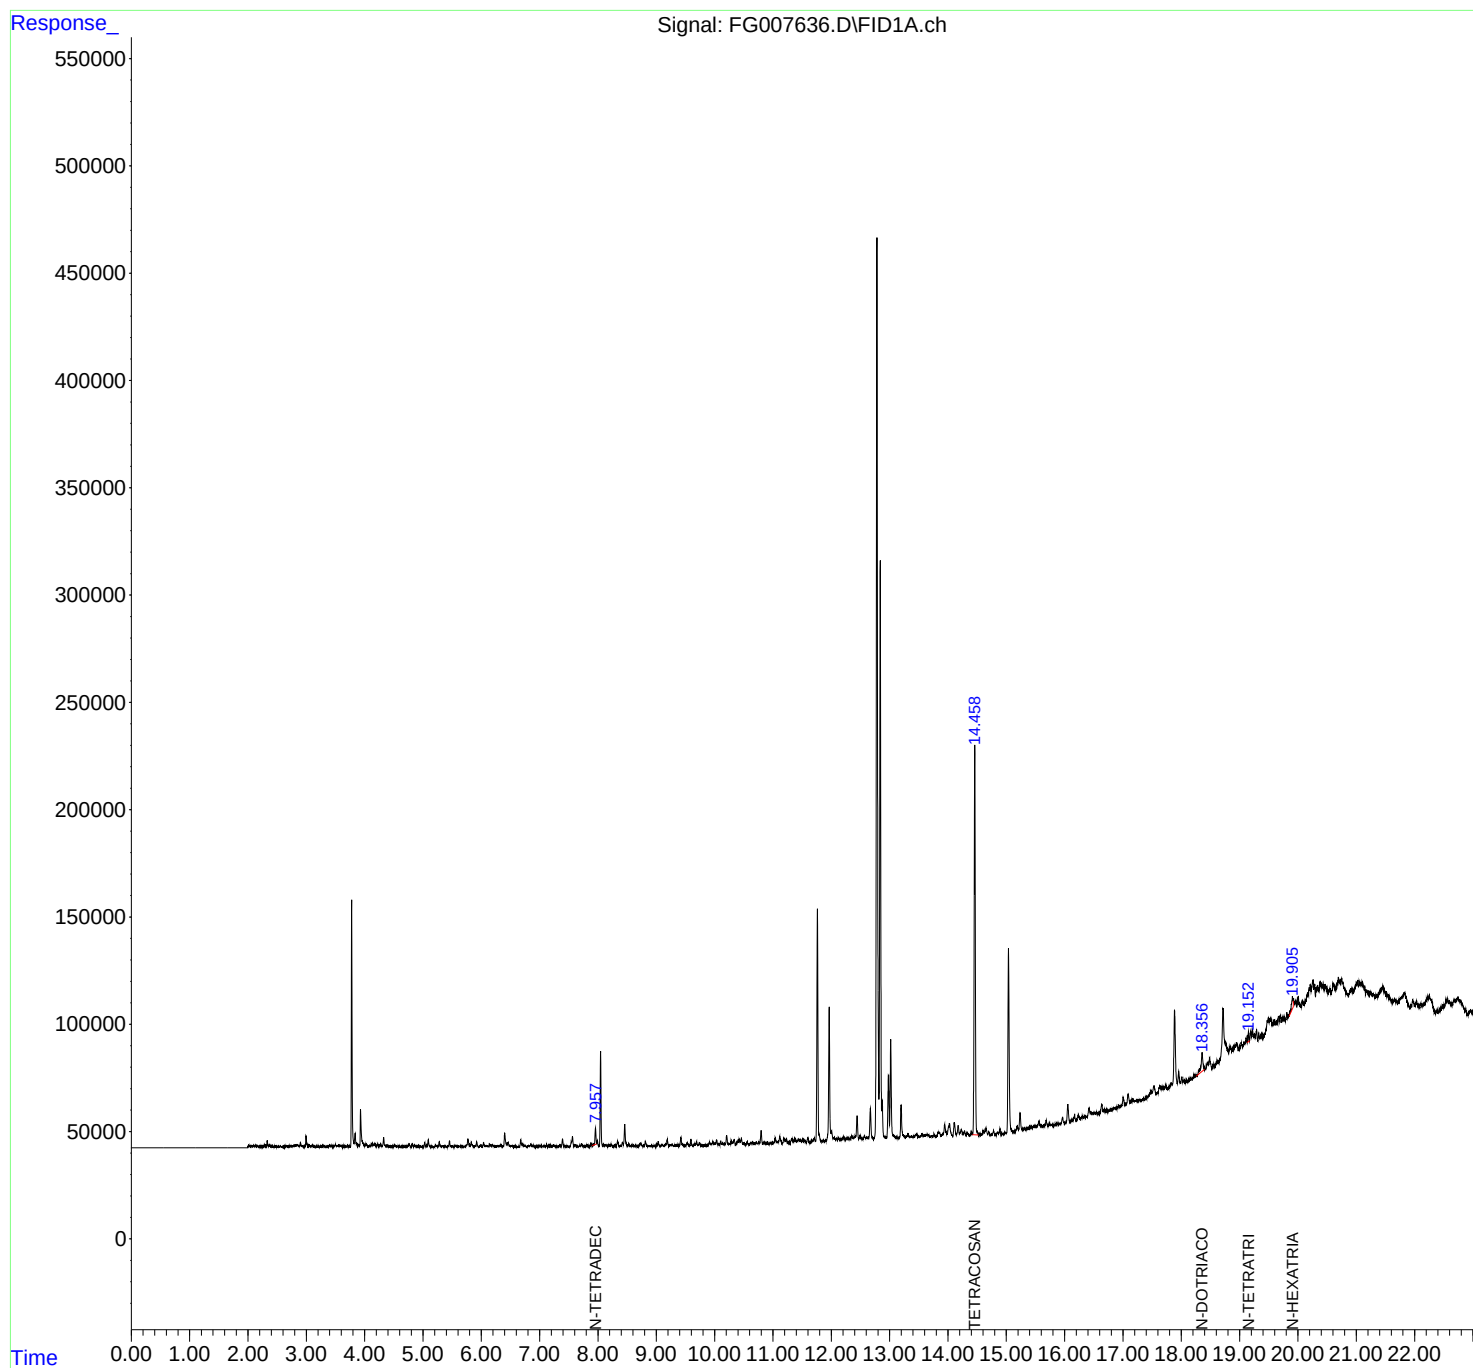


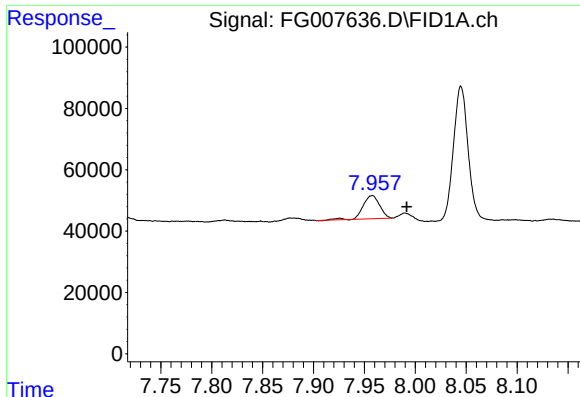

#4 N-TETRADECANE


R.T.: 7.958 min
Delta R.T.: -0.034 min
Response: 86124
Conc: 0.53 ug/ml

Instrument :
FID_G
ClientSampleId :

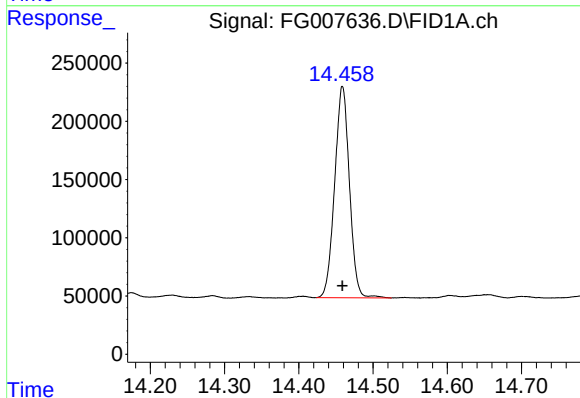


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.459 min
Delta R.T.: 0.000 min
Response: 2510085
Conc: 18.83 ug/ml

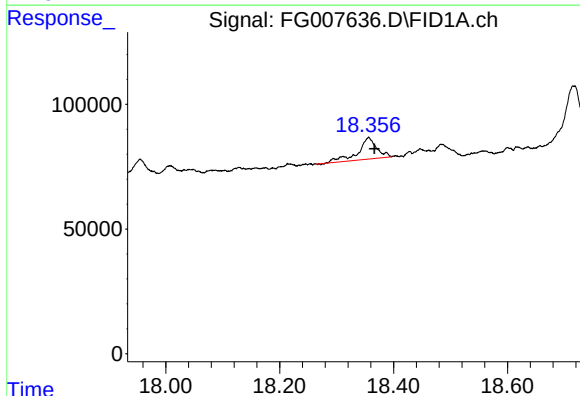


#14 N-DOTRIACONTANE

R.T.: 18.356 min
Delta R.T.: -0.010 min
Response: 195313
Conc: 1.52 ug/ml

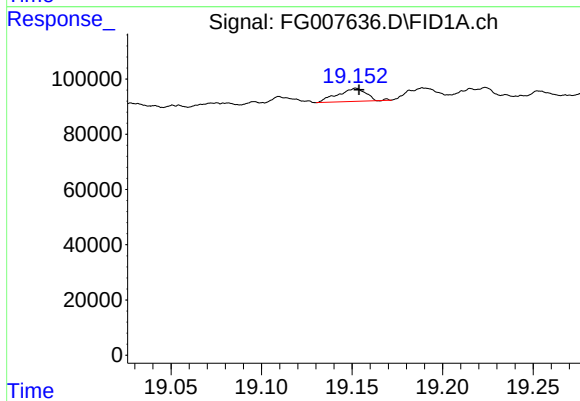

#15 N-TETRATRIACONTANE

R.T.: 19.152 min
Delta R.T.: -0.002 min
Response: 51220
Conc: 0.43 ug/ml

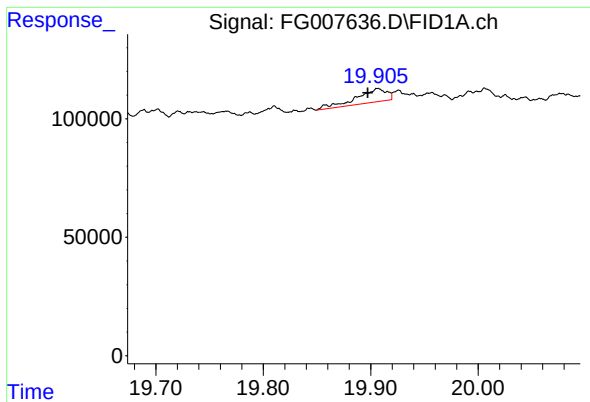

#16 N-HEXATRIACONTANE

R.T.: 19.907 min
Delta R.T.: 0.010 min
Response: 110359
Conc: 0.97 ug/ml

Instrument :
FID_G
ClientSampleId :