

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030619\
Data File : FG004059.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2019 12:14
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 07 00:00:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.192	2998793	22.120 ug/ml
12) N-OCTACOSANE	16.611	2934346	21.433 ug/ml
14) N-DOTRIACONTANE	18.350	427958	3.382 ug/ml
16) N-HEXATRIACONTANE	19.906	764934	6.910 ug/ml
18) N-TETRACONTANE	21.448	1045101	9.854 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030619\
Data File : FG004059.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2019 12:14
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 07 00:00:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

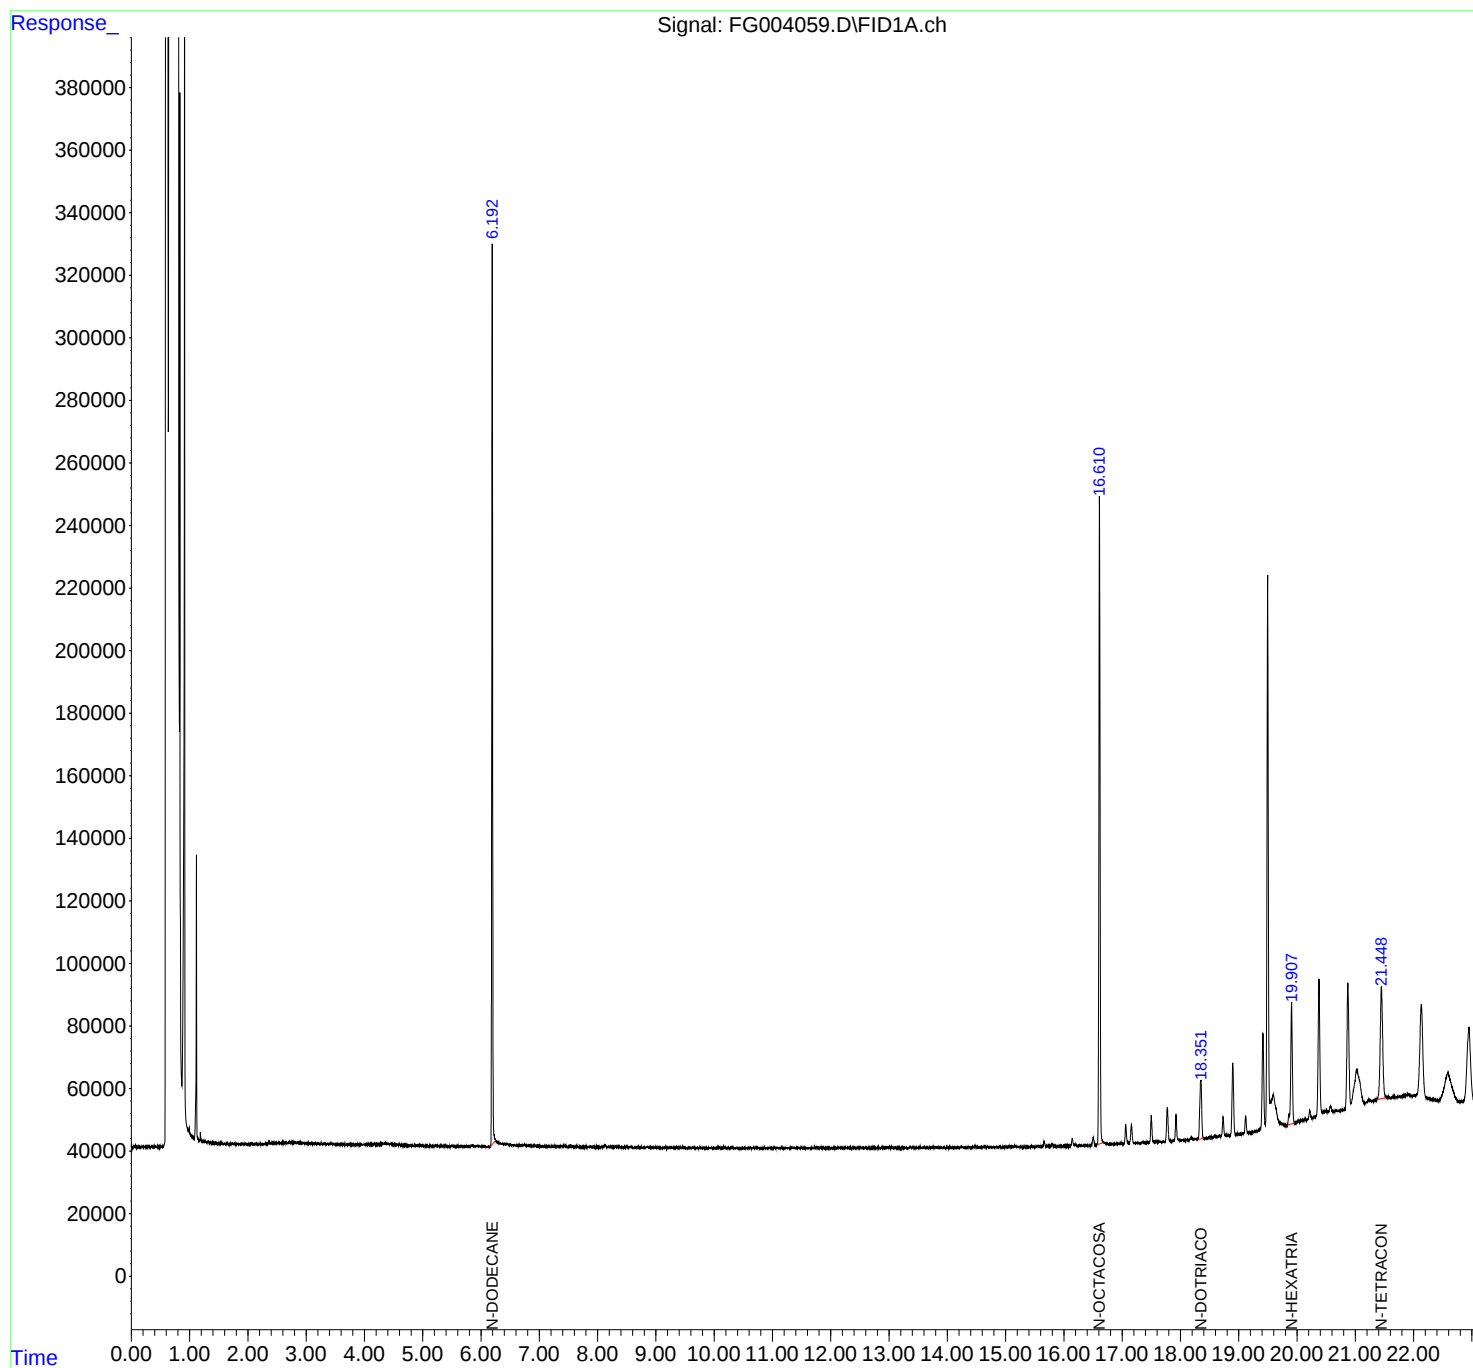


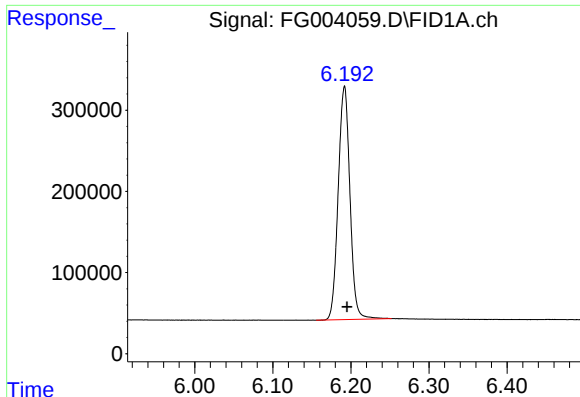

#3 N-DODECANE


R.T.: 6.192 min
Delta R.T.: -0.003 min
Response: 2998793
Conc: 22.12 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

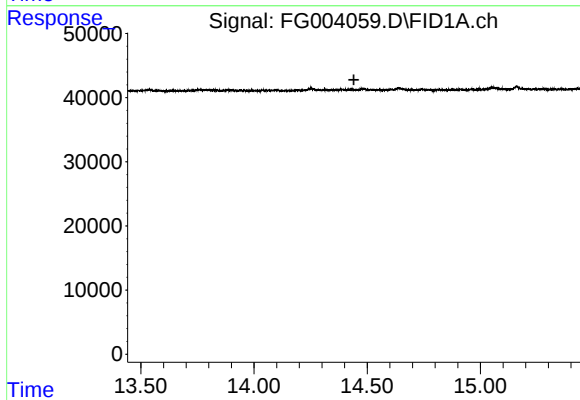


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

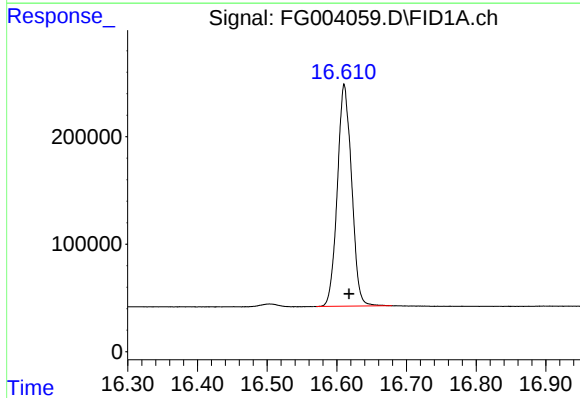


#12 N-OCTACOSANE

R.T.: 16.611 min
Delta R.T.: -0.007 min
Response: 2934346
Conc: 21.43 ug/ml

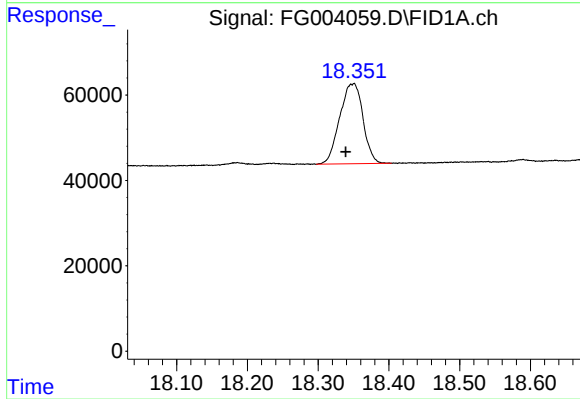

#14 N-DOTRIACONTANE


R.T.: 18.350 min
Delta R.T.: 0.011 min
Response: 427958
Conc: 3.38 ug/ml

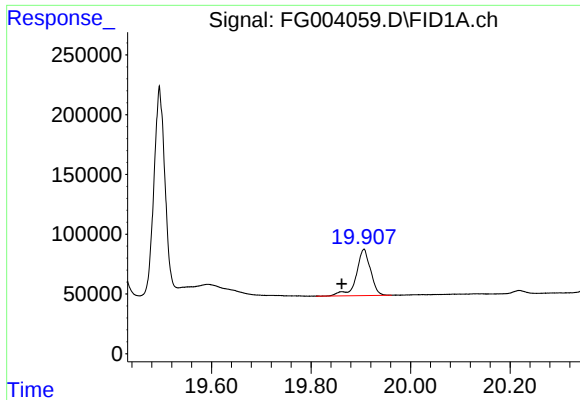

#16 N-HEXATRIACONTANE

R.T.: 19.906 min
Delta R.T.: 0.045 min
Response: 764934
Conc: 6.91 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

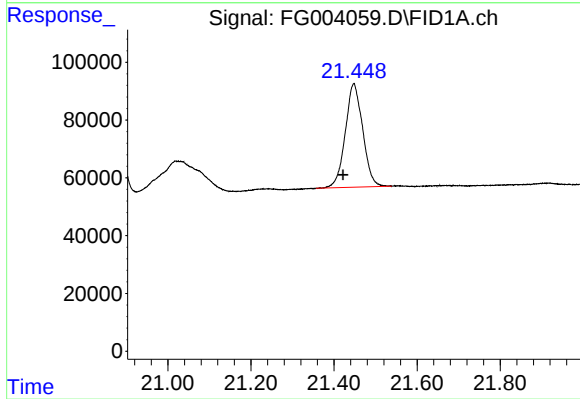

#18 N-TETRACONTANE

R.T.: 21.448 min
Delta R.T.: 0.026 min
Response: 1045101
Conc: 9.85 ug/ml