

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030619\
Data File : FG004060.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2019 12:44
Operator : AJ\SJ
Sample : K1727-01 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-11

Integration File: autoint1.e
Quant Time: Mar 07 00:01:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.170	935408	6.996 ug/ml
3) N-DODECANE	6.191	398147	2.937 ug/ml
4) N-TETRADECANE	7.984	205581	1.474 ug/ml
16) N-HEXATRIACONTANE	19.907	357890	3.233 ug/ml
18) N-TETRACONTANE	21.449	467633	4.409 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030619\
Data File : FG004060.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2019 12:44
Operator : AJ\SJ
Sample : K1727-01 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-11

Integration File: autoint1.e
Quant Time: Mar 07 00:01:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

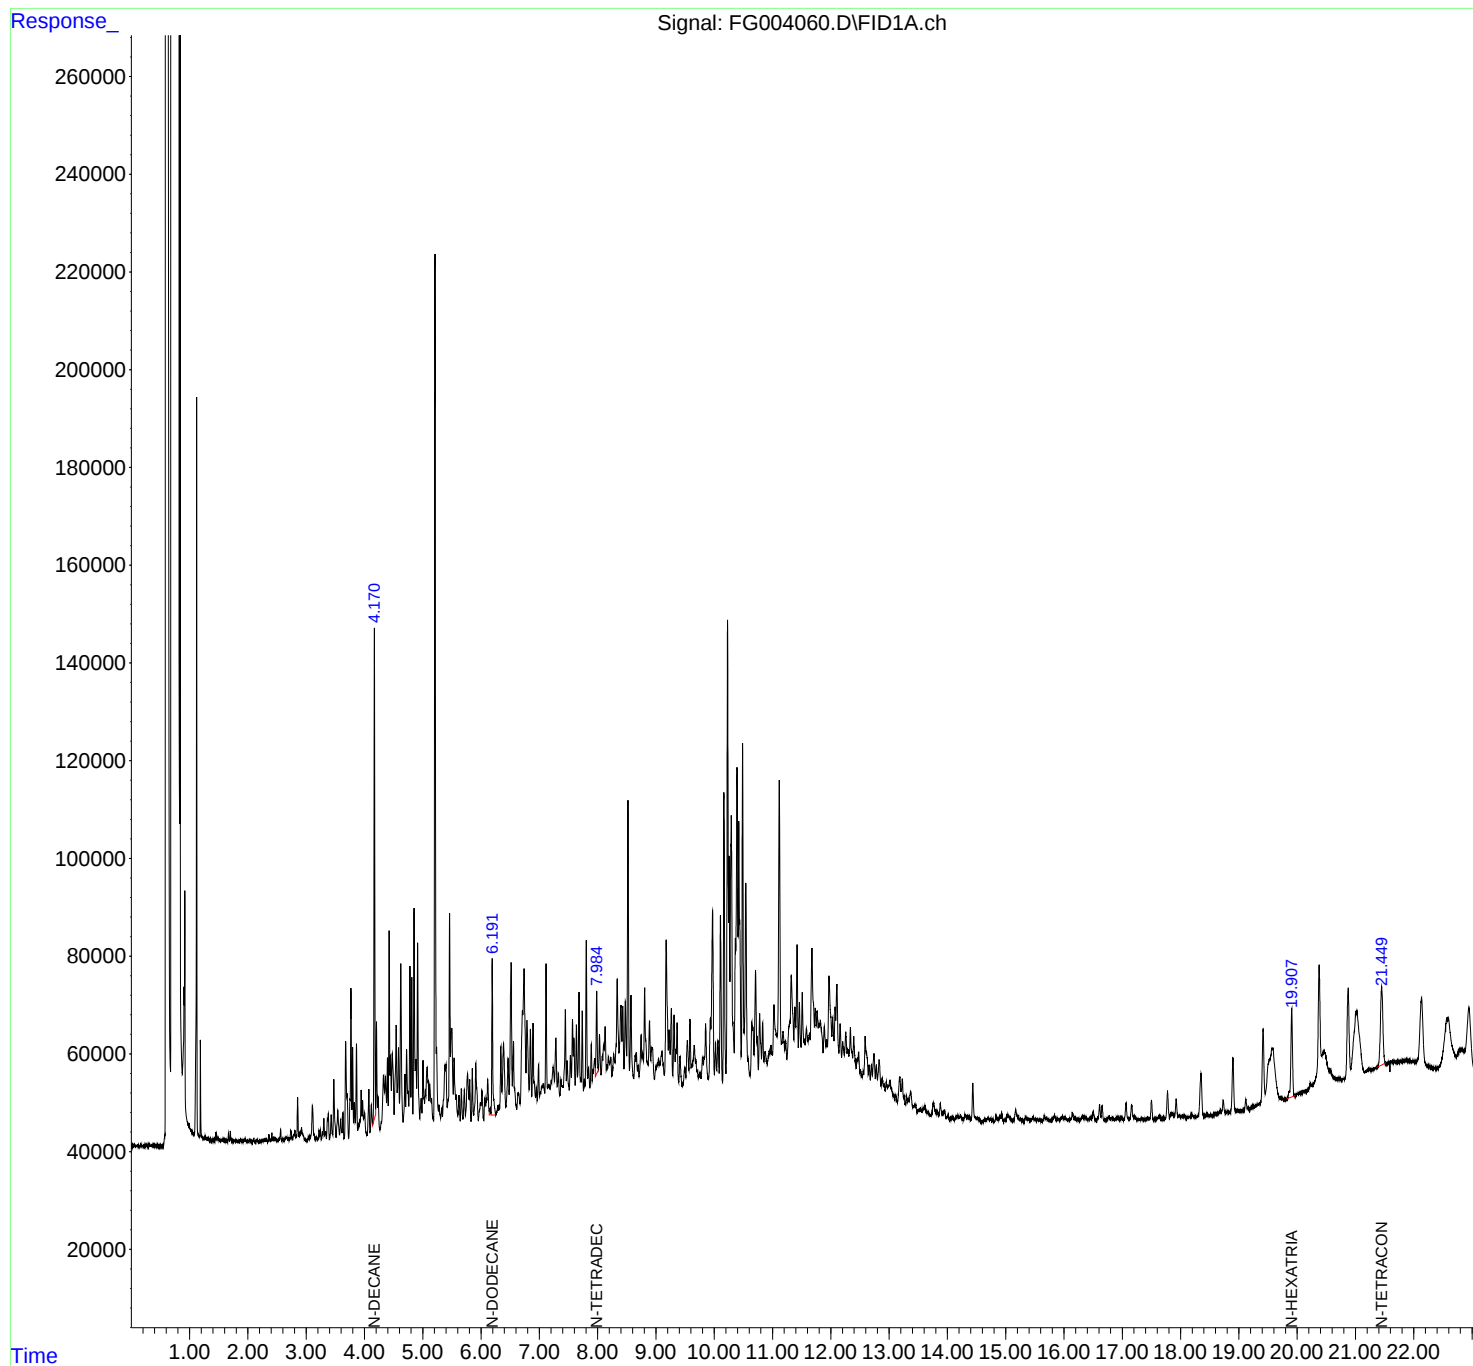


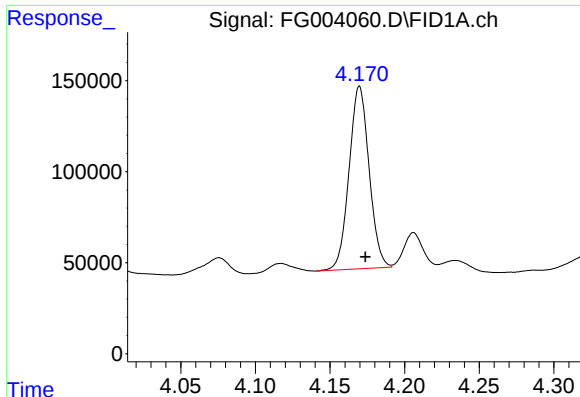

#2 N-DECANE


R.T.: 4.170 min
Delta R.T.: -0.004 min
Response: 935408
Conc: 7.00 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-11

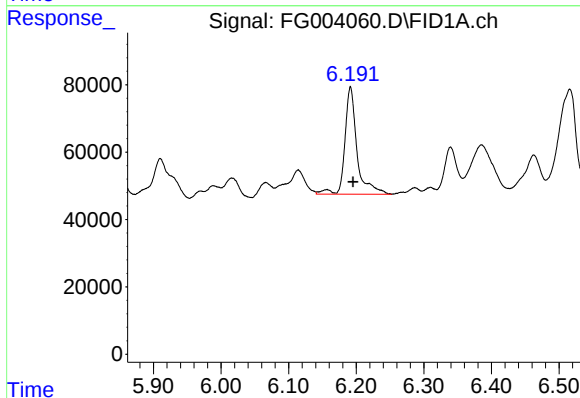


#3 N-DODECANE

R.T.: 6.191 min
Delta R.T.: -0.004 min
Response: 398147
Conc: 2.94 ug/ml

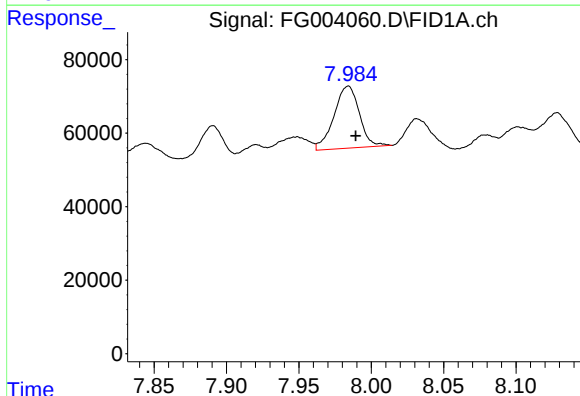


#4 N-TETRADECANE

R.T.: 7.984 min
Delta R.T.: -0.005 min
Response: 205581
Conc: 1.47 ug/ml

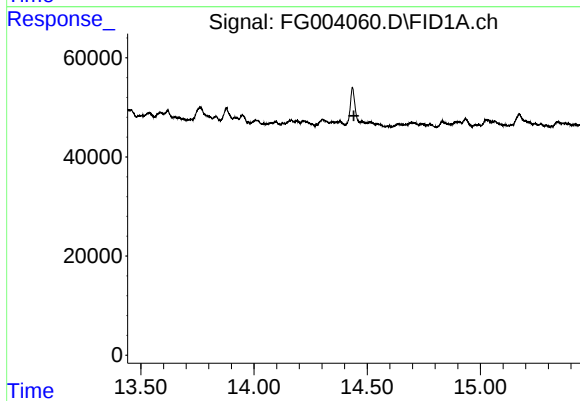

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.441 min
Response: 0
Conc: N.D.

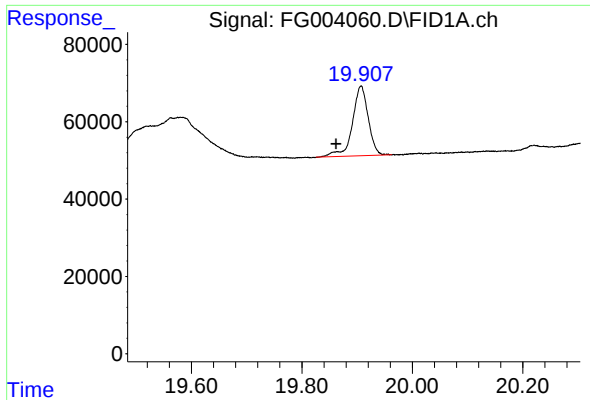

#16 N-HEXATRIACONTANE

R.T.: 19.907 min
Delta R.T.: 0.045 min
Response: 357890
Conc: 3.23 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-11

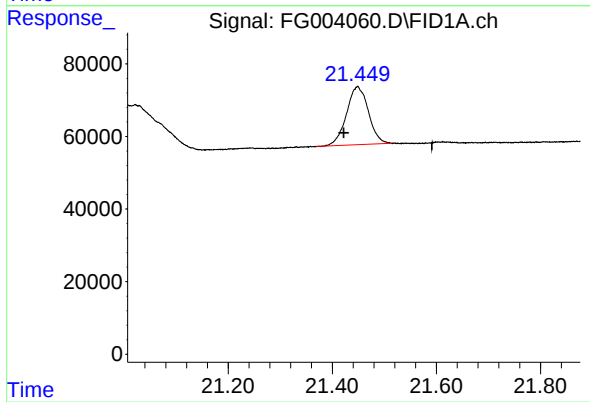

#18 N-TETRACONTANE

R.T.: 21.449 min
Delta R.T.: 0.027 min
Response: 467633
Conc: 4.41 ug/ml