

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030619\
Data File : FG004061.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2019 14:14
Operator : AJ\SJ
Sample : K1727-08 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DUP-1

Integration File: autoint1.e
Quant Time: Mar 07 00:01:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.163	1651329	12.351 ug/ml
3) N-DODECANE	6.186	443385	3.271 ug/ml
4) N-TETRADECANE	7.980	268858	1.928 ug/ml
5) N-HEXADECANE	9.582	142159	0.999 ug/ml
6) N-OCTADECANE	11.023	266600	1.858 ug/ml
14) N-DOTRIACONTANE	18.353	408508	3.229 ug/ml
16) N-HEXATRIACONTANE	19.911	845562	7.638 ug/ml
18) N-TETRACONTANE	21.456	872484	8.226 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030619\
Data File : FG004061.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2019 14:14
Operator : AJ\SJ
Sample : K1727-08 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DUP-1

Integration File: autoint1.e
Quant Time: Mar 07 00:01:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

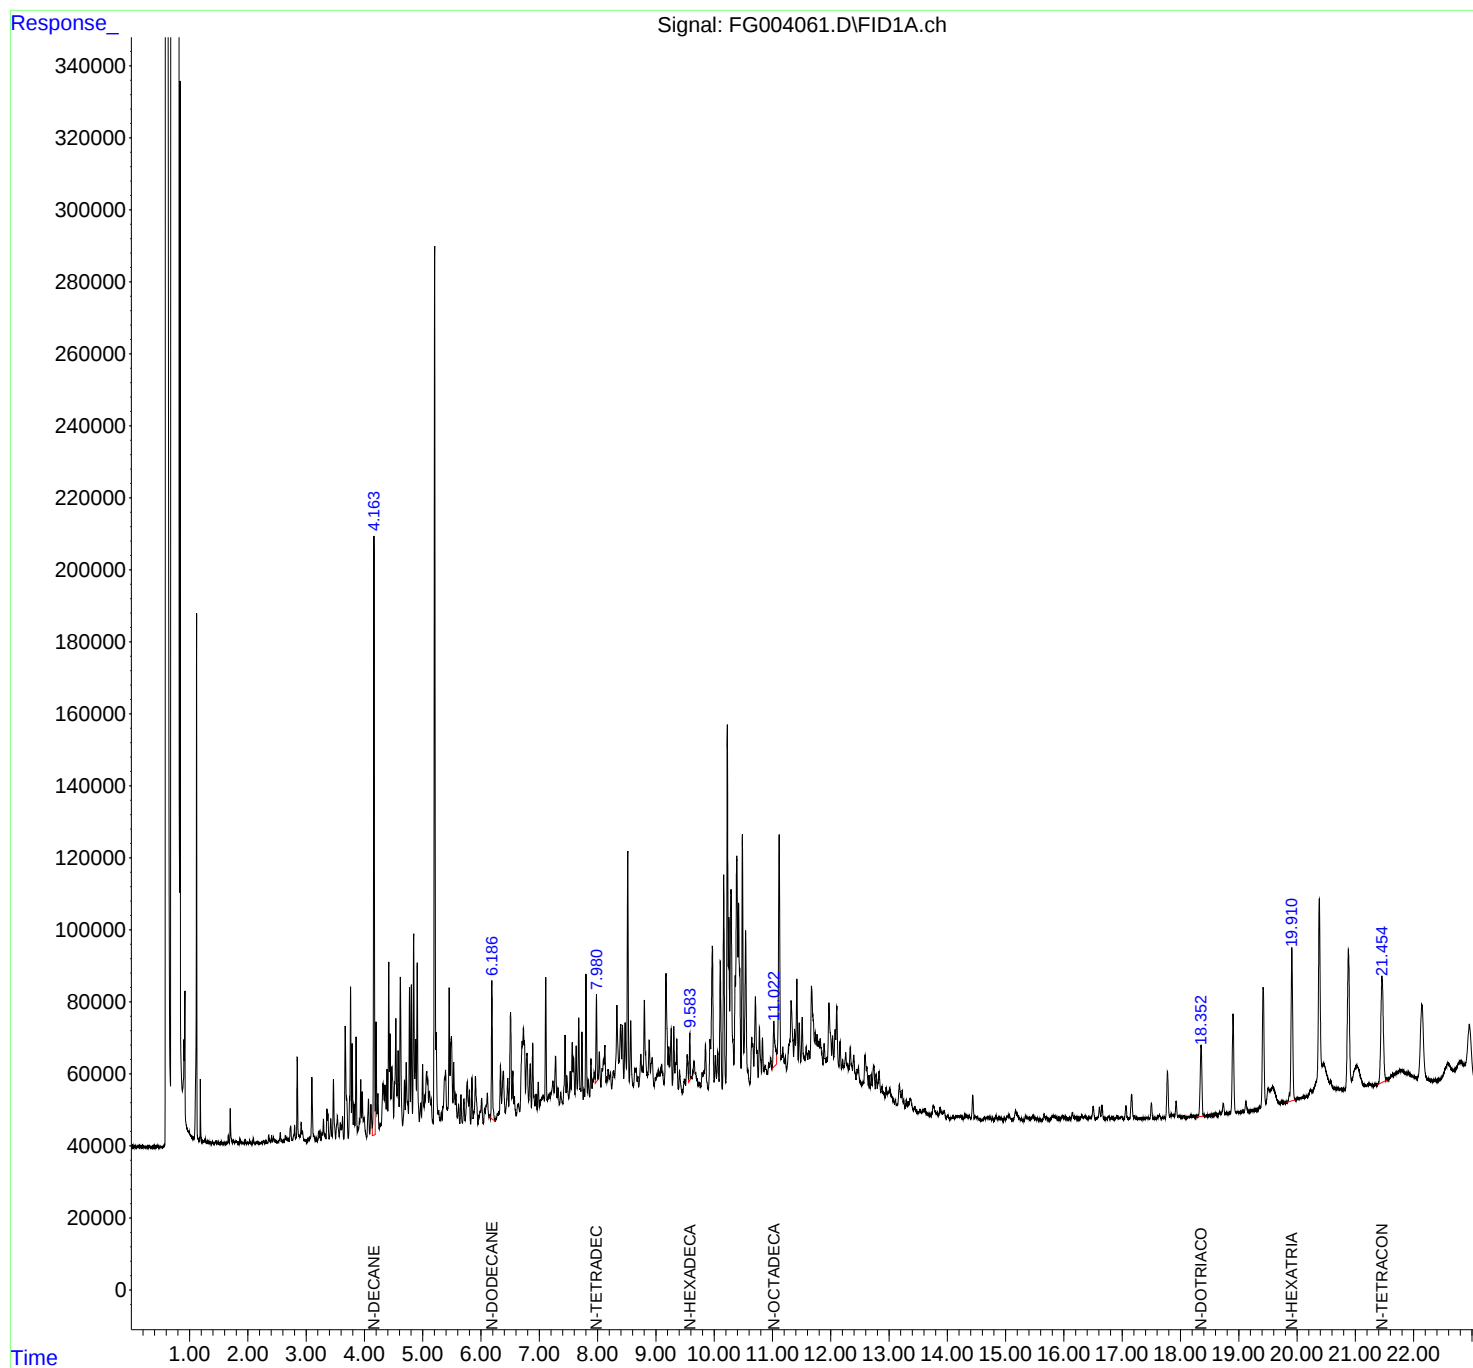


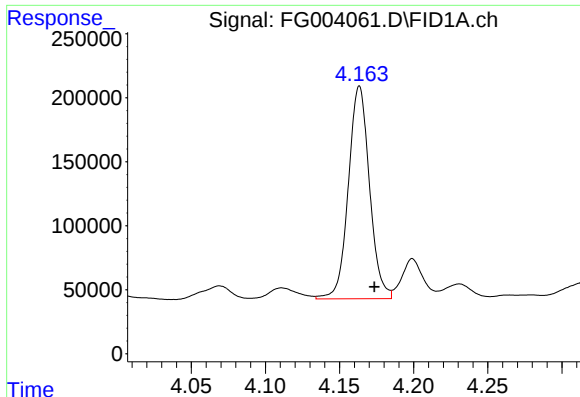

#2 N-DECANE


R.T.: 4.163 min
Delta R.T.: -0.010 min
Response: 1651329
Conc: 12.35 ug/ml

Instrument :
FID_G
ClientSampleId :
DUP-1

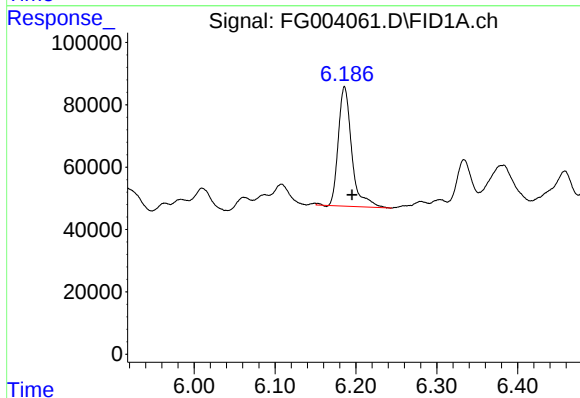


#3 N-DODECANE

R.T.: 6.186 min
Delta R.T.: -0.009 min
Response: 443385
Conc: 3.27 ug/ml

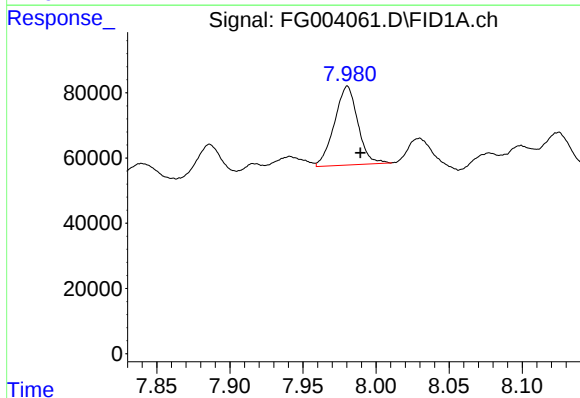


#4 N-TETRADECANE

R.T.: 7.980 min
Delta R.T.: -0.009 min
Response: 268858
Conc: 1.93 ug/ml

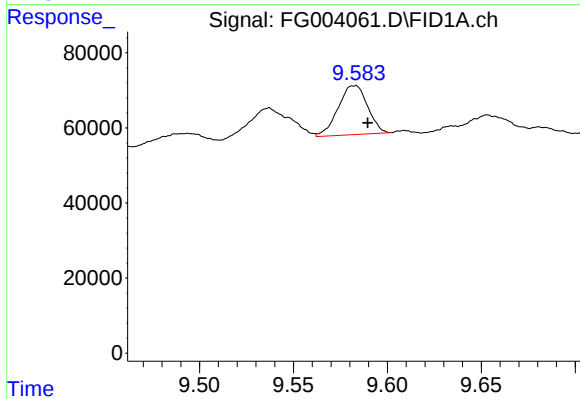

#5 N-HEXADECANE


R.T.: 9.582 min
Delta R.T.: -0.007 min
Response: 142159
Conc: 1.00 ug/ml

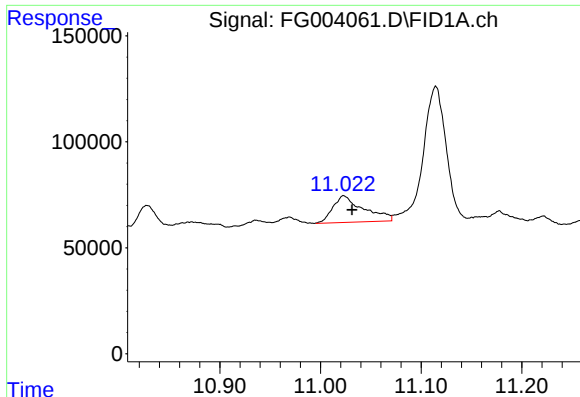

#6 N-OCTADECANE


R.T.: 11.023 min
Delta R.T.: -0.008 min
Response: 266600
Conc: 1.86 ug/ml

Instrument :
FID_G
ClientSampleId :
DUP-1

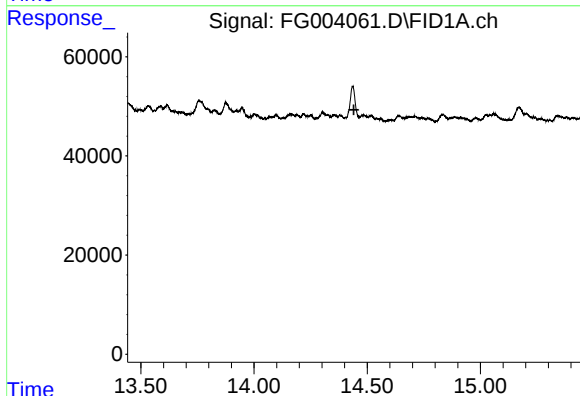


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

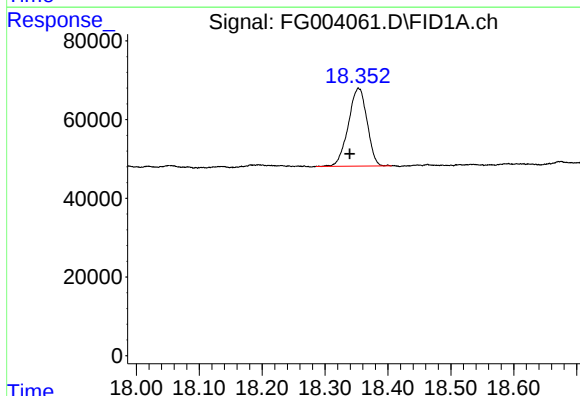


#14 N-DOTRIACONTANE

R.T.: 18.353 min
Delta R.T.: 0.014 min
Response: 408508
Conc: 3.23 ug/ml

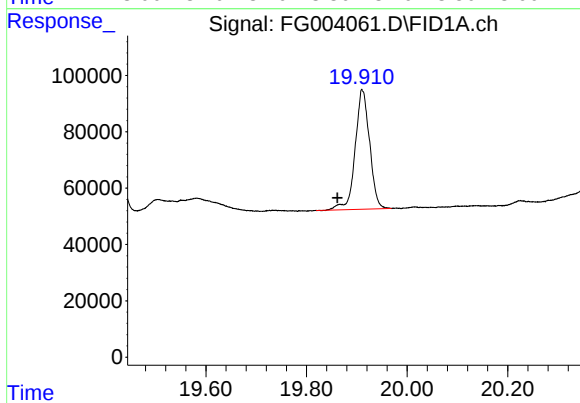

#16 N-HEXATRIACONTANE

R.T.: 19.911 min
Delta R.T.: 0.049 min
Response: 845562
Conc: 7.64 ug/ml

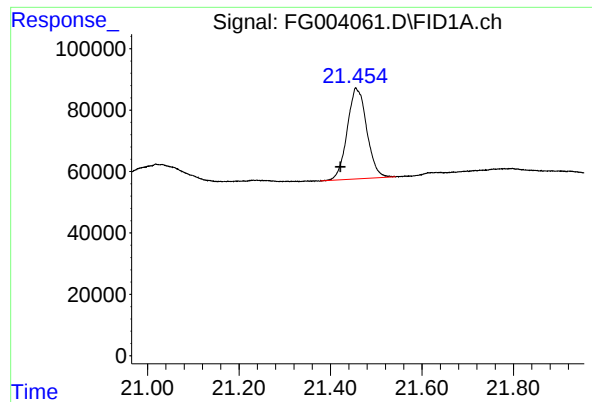

#18 N-TETRACONTANE

R.T.: 21.456 min
Delta R.T.: 0.034 min
Response: 872484
Conc: 8.23 ug/ml

Instrument :
FID_G
ClientSampleId :
DUP-1