

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030623\
Data File : FG011526.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2023 09:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 07 02:40:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.065	2073950	19.718 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.133	47607	0.449 ug/ml
14) N-DOTRIACONTANE	18.968	58770	0.582 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030623\
Data File : FG011526.D
Signal(s) : FID1A.ch
Acq On : 06 Mar 2023 09:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 07 02:40:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

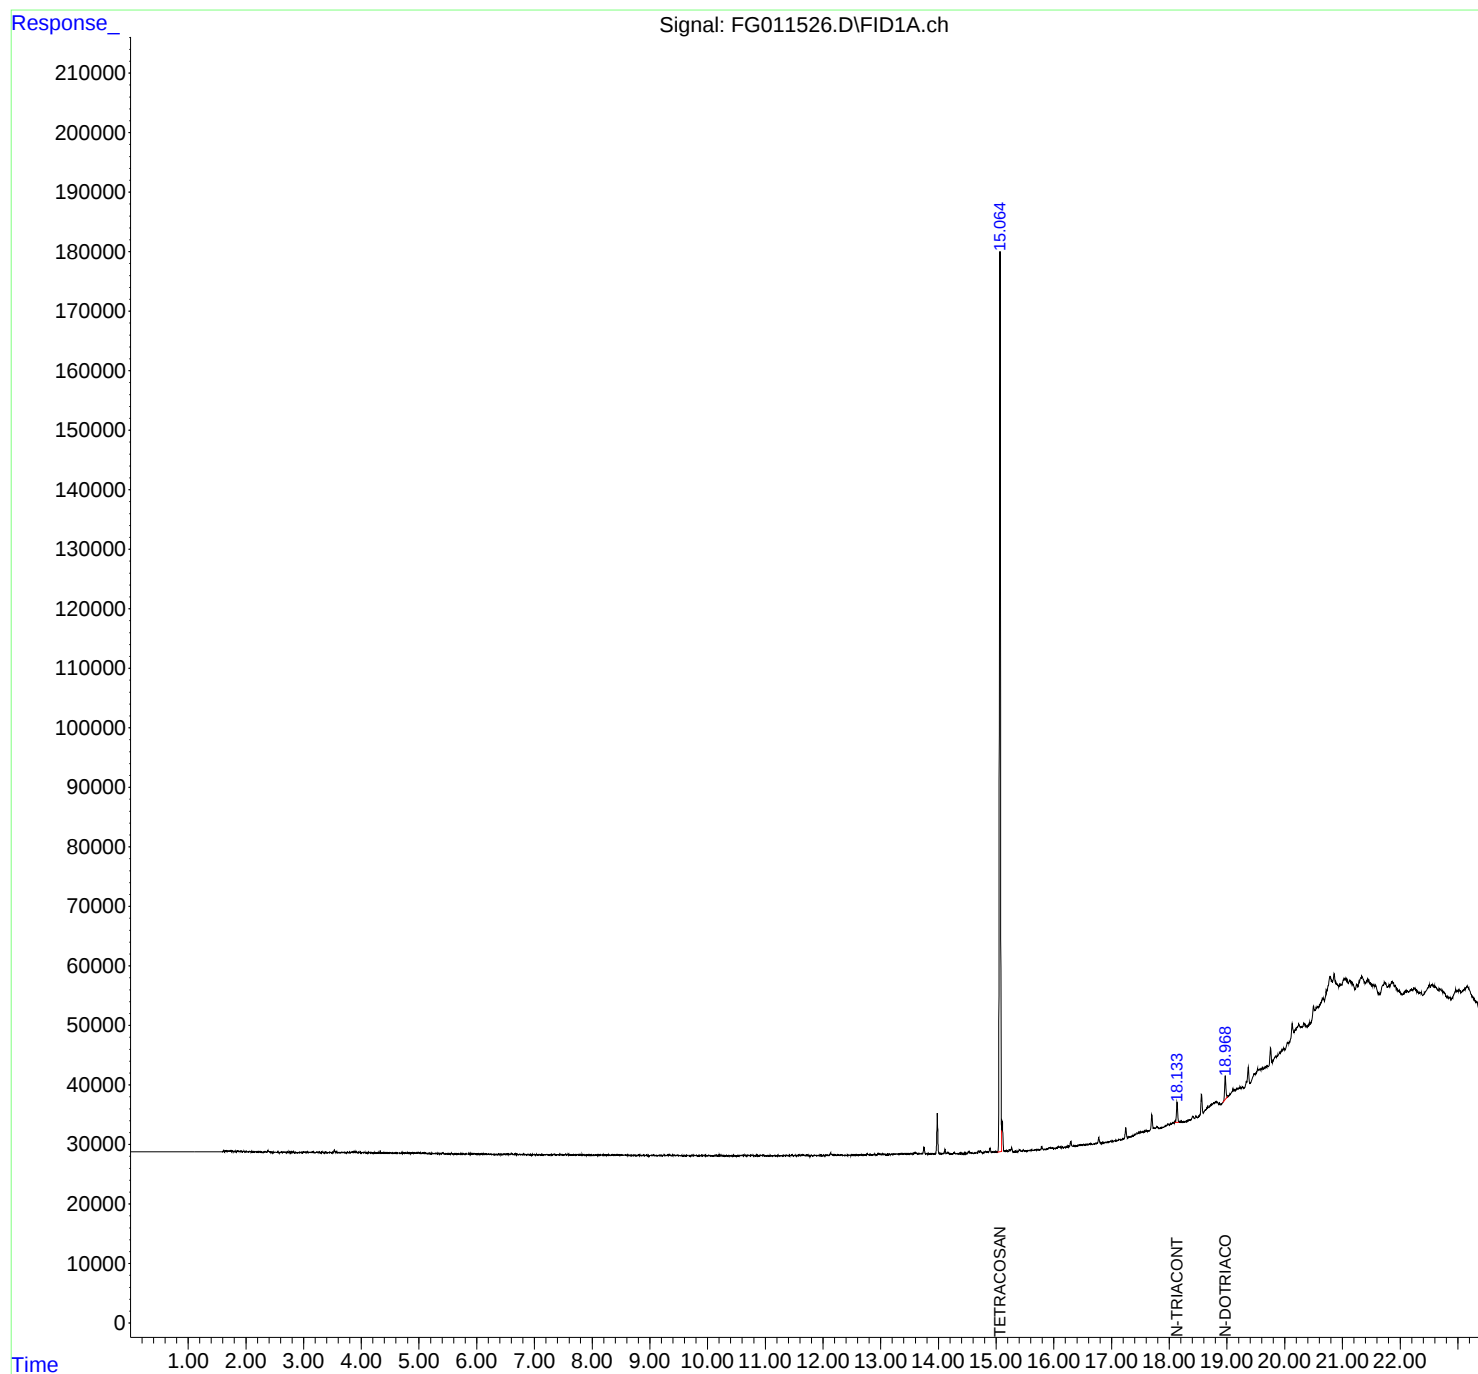

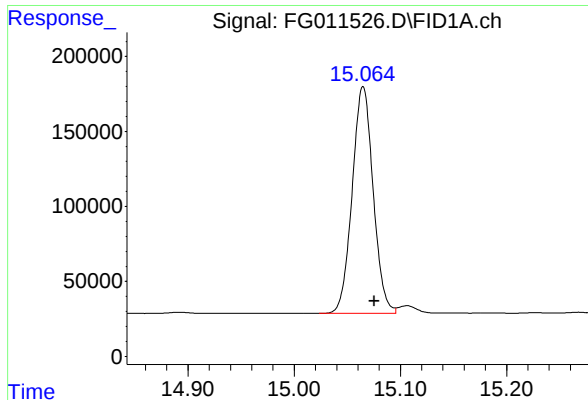


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.065 min
Delta R.T.: -0.011 min
Response: 2073950
Conc: 19.72 ug/ml

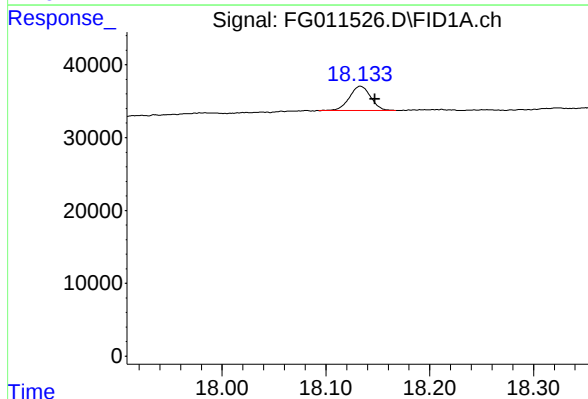

#13 N-TRIACONTANE

R.T.: 18.133 min
Delta R.T.: -0.014 min
Response: 47607
Conc: 0.45 ug/ml

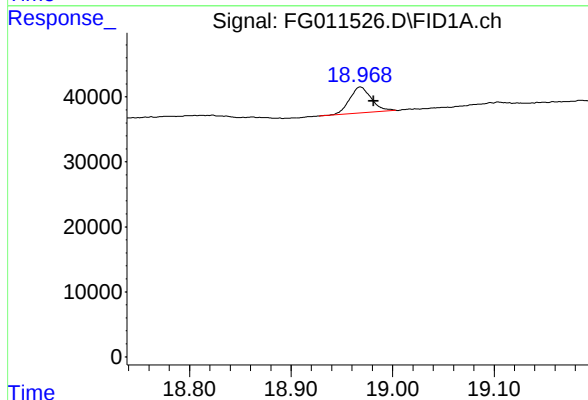

#14 N-DOTRIACONTANE

R.T.: 18.968 min
Delta R.T.: -0.013 min
Response: 58770
Conc: 0.58 ug/ml