

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030719\
 Data File : FG004073.D
 Signal(s) : FID1A.ch
 Acq On : 07 Mar 2019 16:15
 Operator : AJ\SJ
 Sample : K1757-02MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 08 00:38:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.168	2162941	16.178 ug/ml
3) N-DODECANE	6.190	2400218	17.705 ug/ml
4) N-TETRADECANE	7.983	2617742	18.773 ug/ml
5) N-HEXADECANE	9.583	2821984	19.829 ug/mlm
6) N-OCTADECANE	11.026	2788873	19.438 ug/ml
7) N-EICOSANE	12.337	2752155	19.265 ug/ml
8) N-DOCOSANE	13.534	2803181	19.749 ug/mlm
10) N-TETRACOSANE	14.637	2768122	19.628 ug/ml
11) N-HEXACOSANE	15.660	2603179	18.691 ug/ml
12) N-OCTACOSANE	16.611	2672145	19.518 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030719\
Data File : FG004073.D
Signal(s) : FID1A.ch
Acq On : 07 Mar 2019 16:15
Operator : AJ\SJ
Sample : K1757-02MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 08 00:38:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

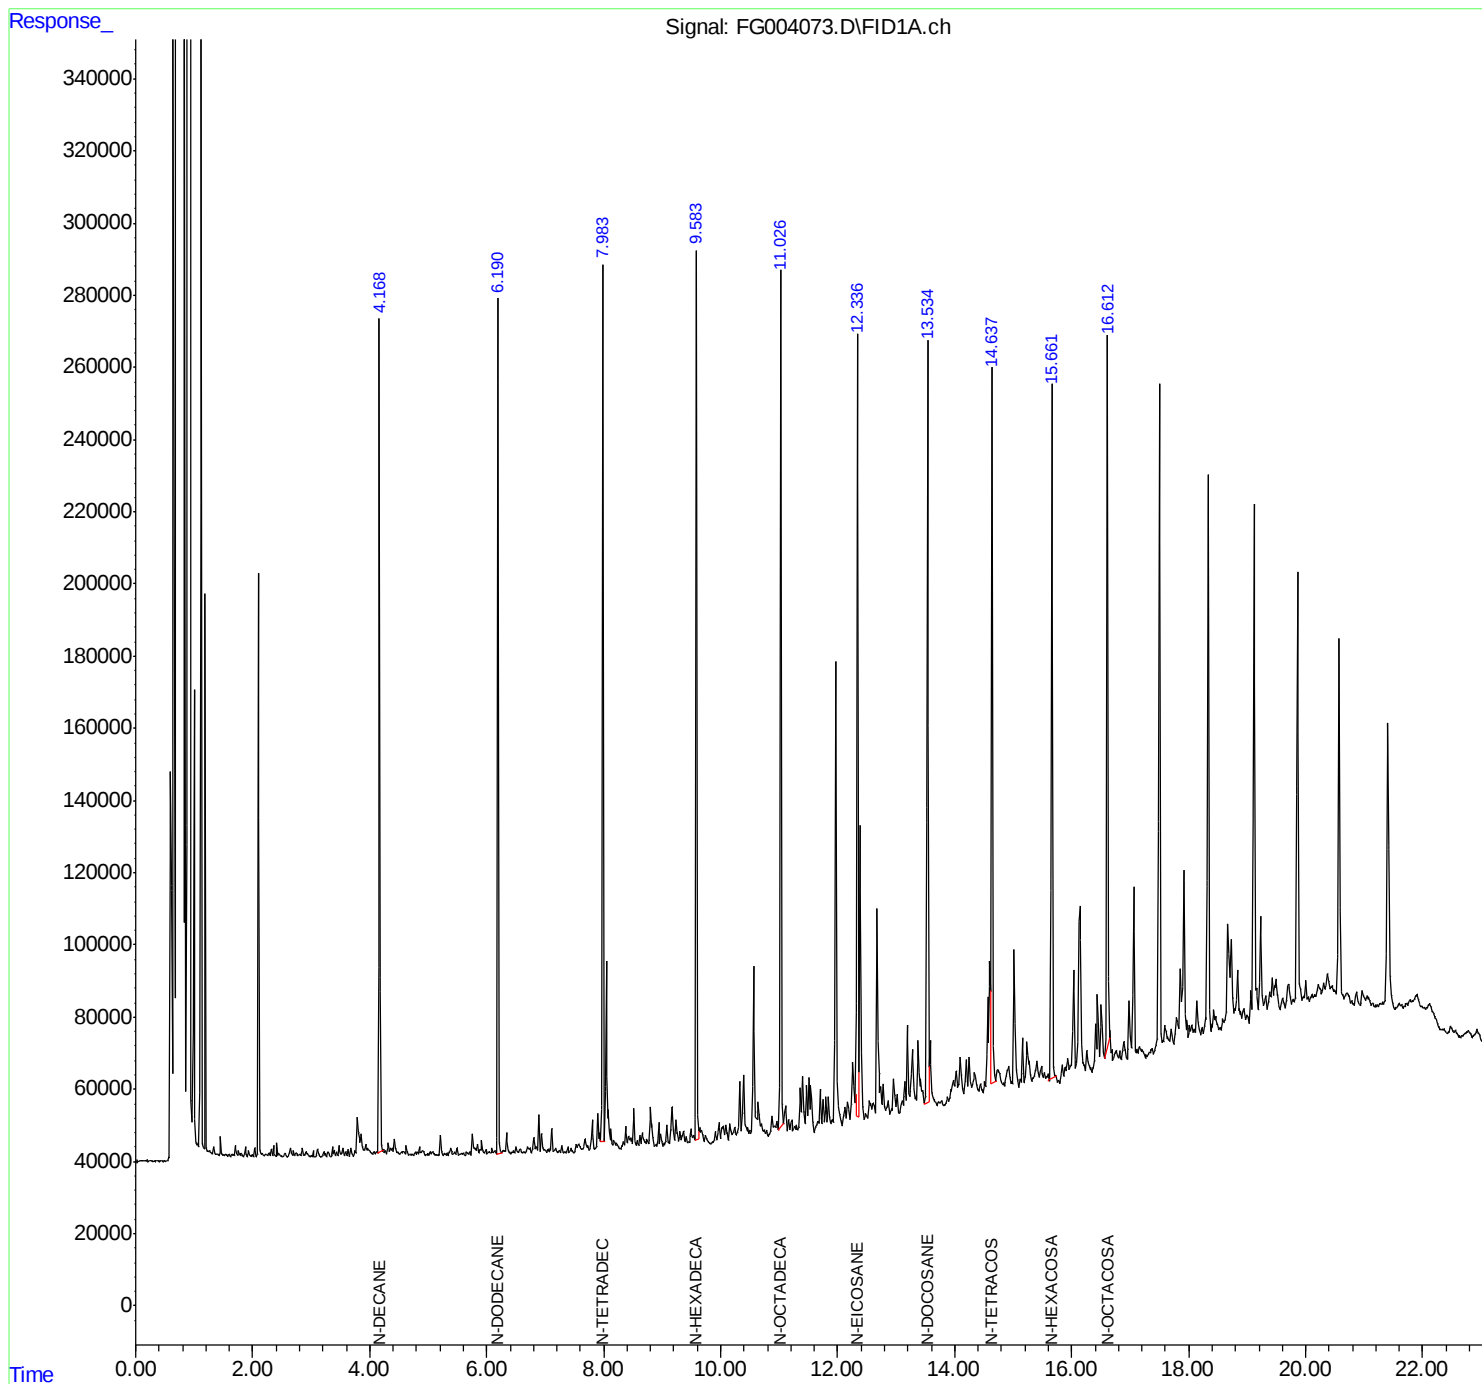

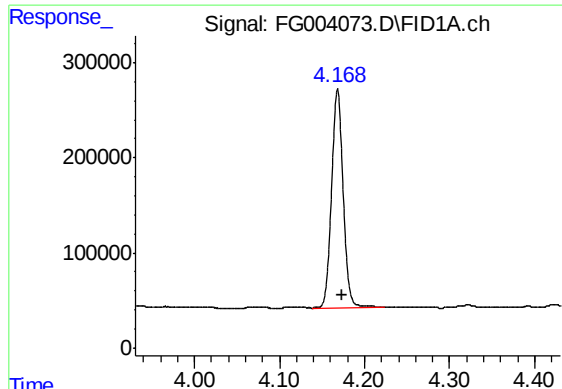


#2 N-DECANE

R.T.: 4.168 min
Delta R.T.: -0.005 min
Response: 2162941
Conc: 16.18 ug/ml

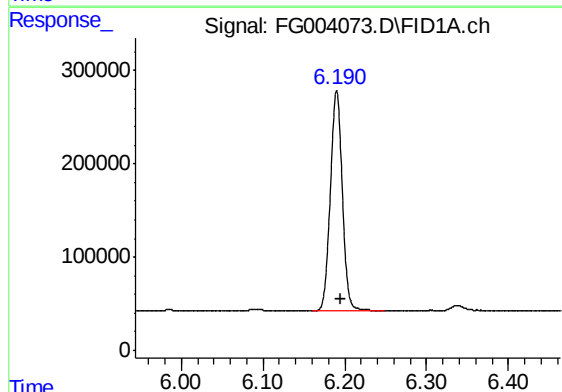


#3 N-DODECANE

R.T.: 6.190 min
Delta R.T.: -0.005 min
Response: 2400218
Conc: 17.70 ug/ml

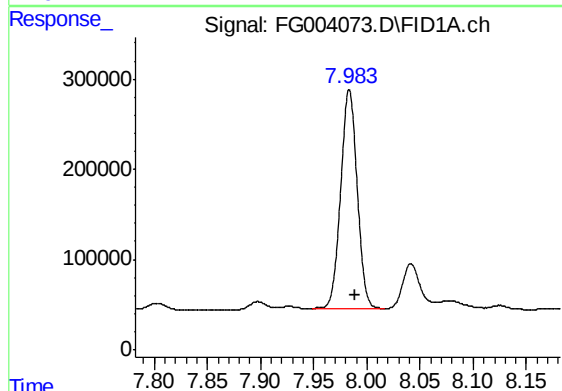


#4 N-TETRADECANE

R.T.: 7.983 min
Delta R.T.: -0.006 min
Response: 2617742
Conc: 18.77 ug/ml

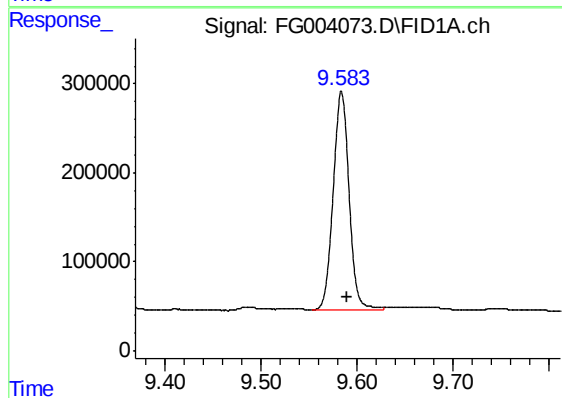


#5 N-HEXADECANE

R.T.: 9.583 min
Delta R.T.: -0.007 min
Response: 2821984
Conc: 19.83 ug/ml m

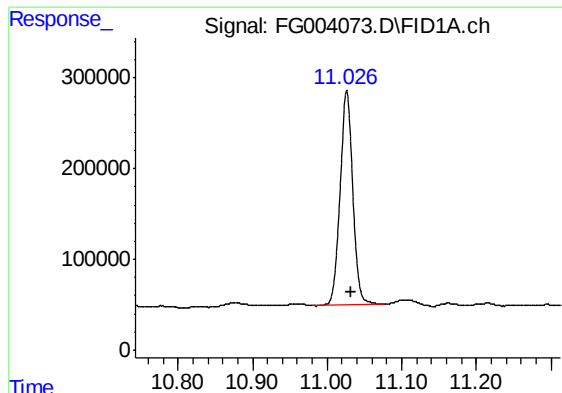


#6 N-OCTADECANE

R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 2788873
Conc: 19.44 ug/ml

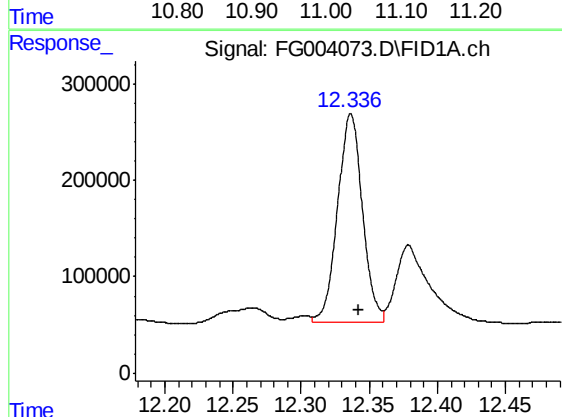


#7 N-EICOSANE

R.T.: 12.337 min
Delta R.T.: -0.006 min
Response: 2752155
Conc: 19.27 ug/ml

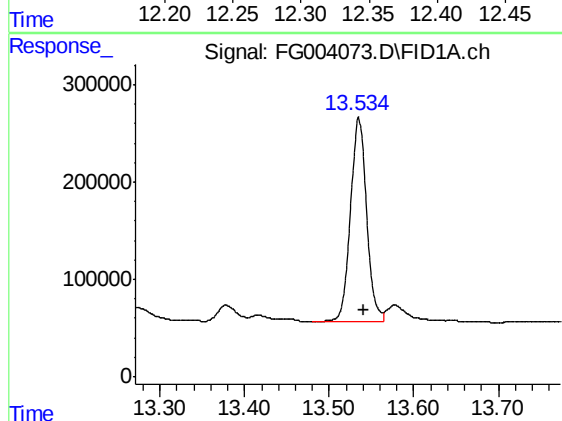


#8 N-DOCOSANE

R.T.: 13.534 min
Delta R.T.: -0.007 min
Response: 2803181
Conc: 19.75 ug/ml m

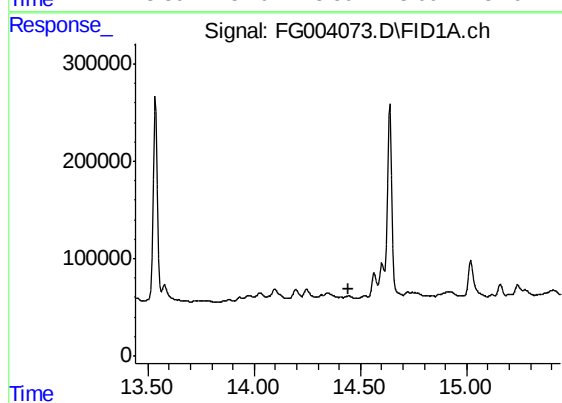


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.441 min
Response: 0
Conc: N.D.

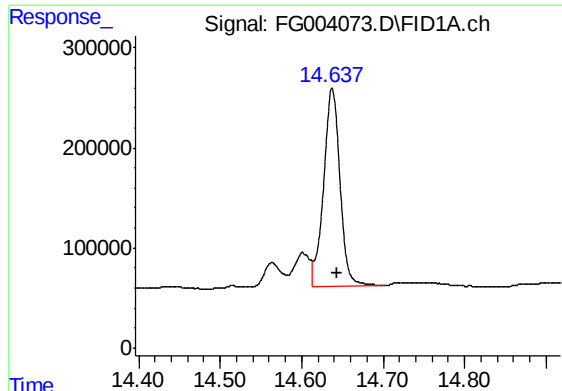


#10 N-TETRACOSANE

R.T.: 14.637 min
Delta R.T.: -0.006 min
Response: 2768122
Conc: 19.63 ug/ml

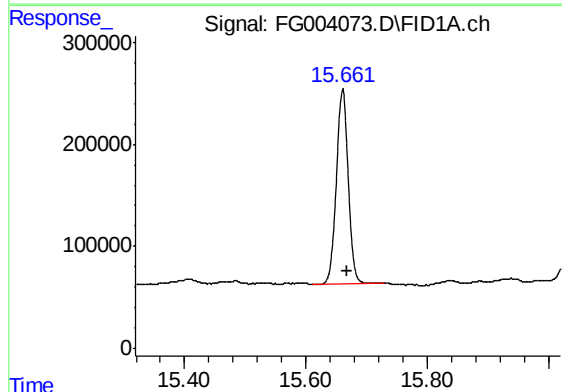

#11 N-HEXACOSANE

R.T.: 15.660 min
Delta R.T.: -0.007 min
Response: 2603179
Conc: 18.69 ug/ml

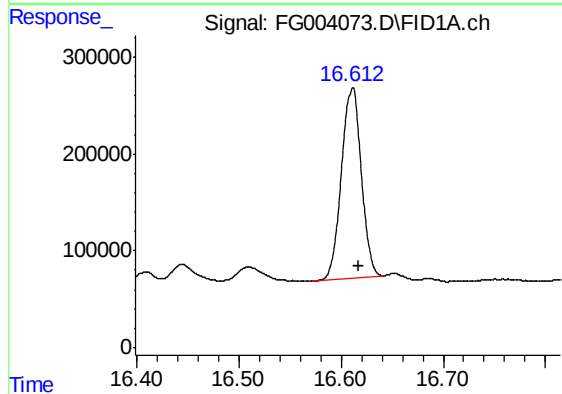

#12 N-OCTACOSANE

R.T.: 16.611 min
Delta R.T.: -0.006 min
Response: 2672145
Conc: 19.52 ug/ml