

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030719\
 Data File : FG004088.D
 Signal(s) : FID1A.ch
 Acq On : 07 Mar 2019 23:44
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 08 00:41:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.436	6078951	48.353 ug/ml
Target Compounds			
2) N-DECANE	4.170	7783411	58.216 ug/ml
3) N-DODECANE	6.193	7741790	57.107 ug/ml
4) N-TETRADECANE	7.987	7696002	55.190 ug/ml
5) N-HEXADECANE	9.587	7622994	53.563 ug/ml
6) N-OCTADECANE	11.028	7524523	52.445 ug/ml
7) N-EICOSANE	12.338	7319306	51.236 ug/ml
8) N-DOCOSANE	13.535	7061495	49.750 ug/ml
10) N-TETRACOSANE	14.640	6790871	48.152 ug/ml
11) N-HEXACOSANE	15.661	6533758	46.913 ug/ml
12) N-OCTACOSANE	16.611	6362267	46.471 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030719\
Data File : FG004088.D
Signal(s) : FID1A.ch
Acq On : 07 Mar 2019 23:44
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 08 00:41:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

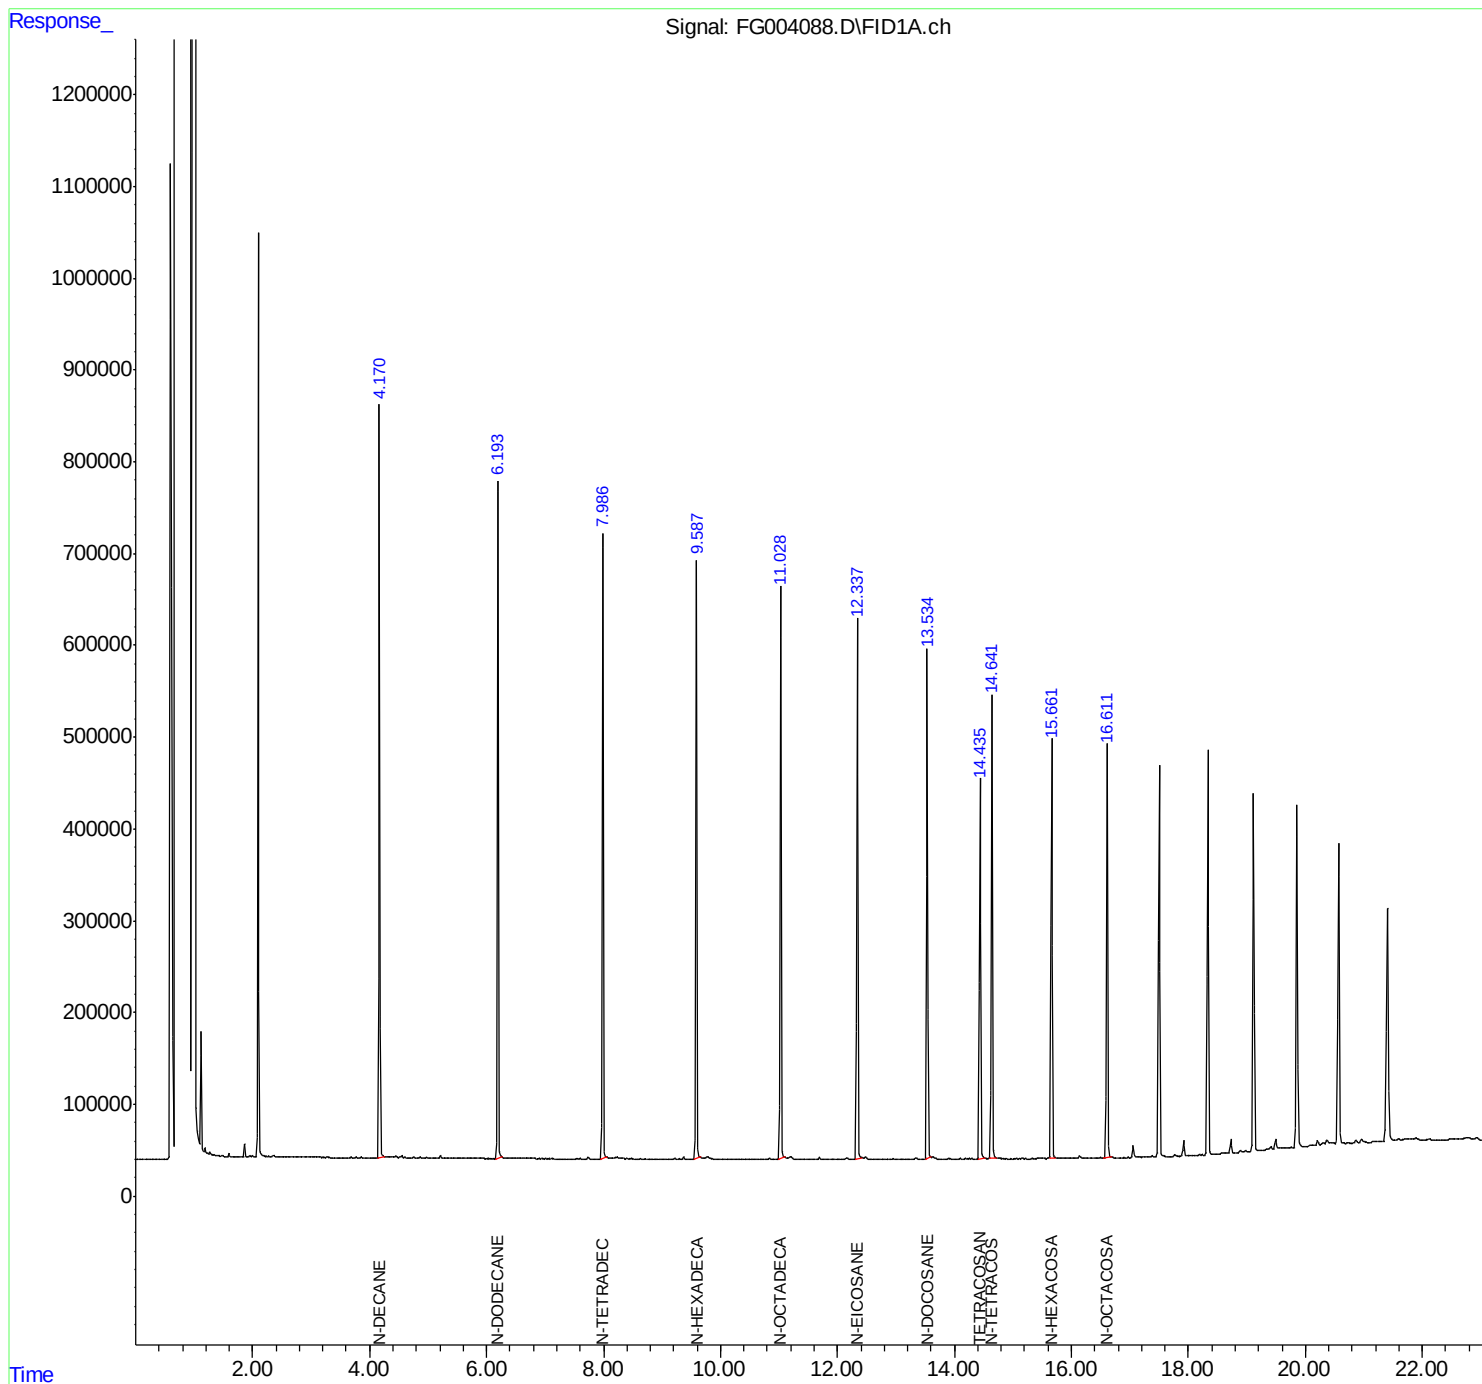

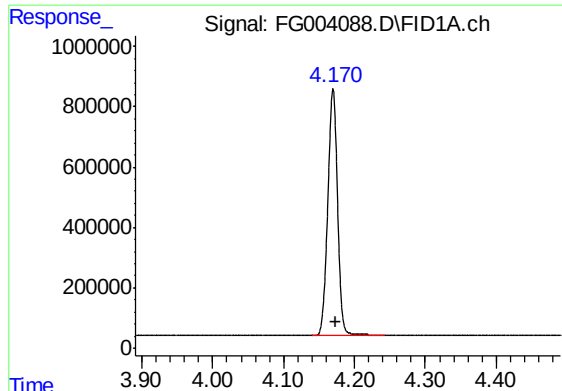


#2 N-DECANE

R.T.: 4.170 min
Delta R.T.: -0.004 min
Response: 7783411
Conc: 58.22 ug/ml

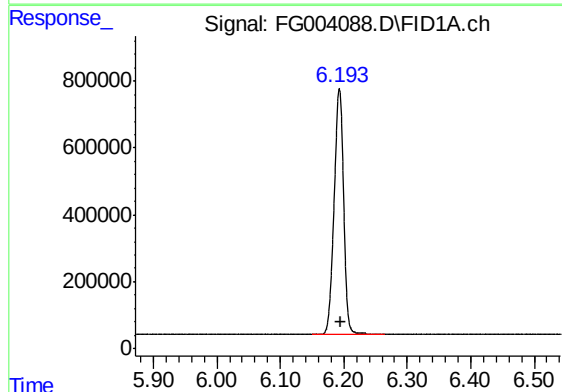


#3 N-DODECANE

R.T.: 6.193 min
Delta R.T.: -0.002 min
Response: 7741790
Conc: 57.11 ug/ml

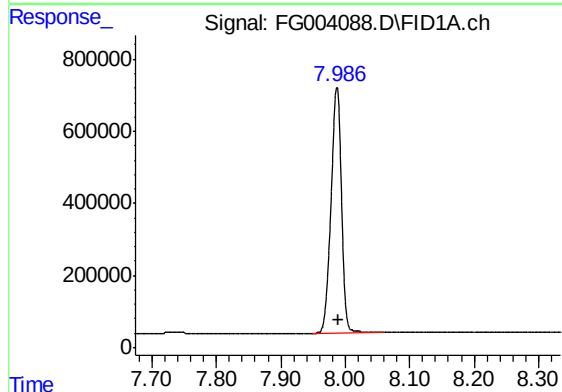


#4 N-TETRADECANE

R.T.: 7.987 min
Delta R.T.: -0.002 min
Response: 7696002
Conc: 55.19 ug/ml

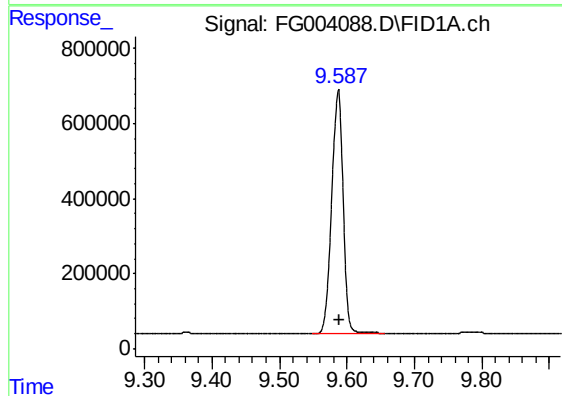


#5 N-HEXADECANE

R.T.: 9.587 min
Delta R.T.: -0.002 min
Response: 7622994
Conc: 53.56 ug/ml

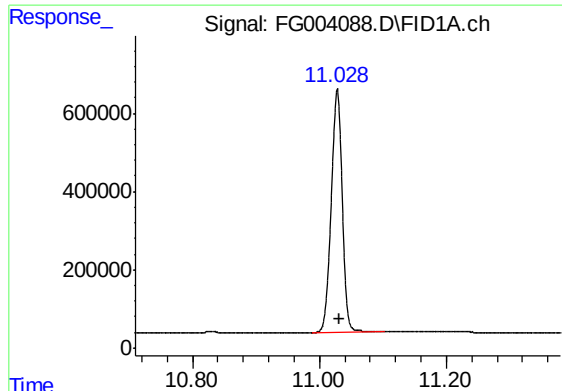


#6 N-OCTADECANE

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 7524523
Conc: 52.44 ug/ml

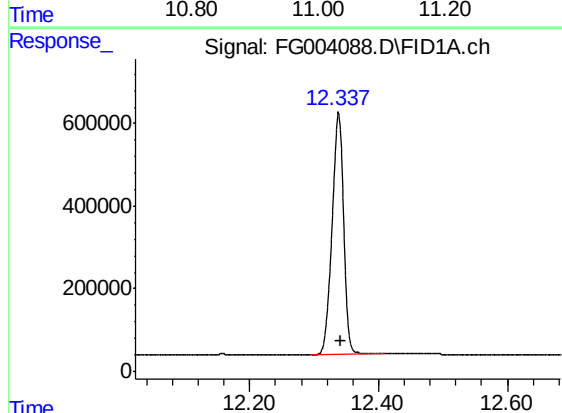


#7 N-EICOSANE

R.T.: 12.338 min
Delta R.T.: -0.005 min
Response: 7319306
Conc: 51.24 ug/ml

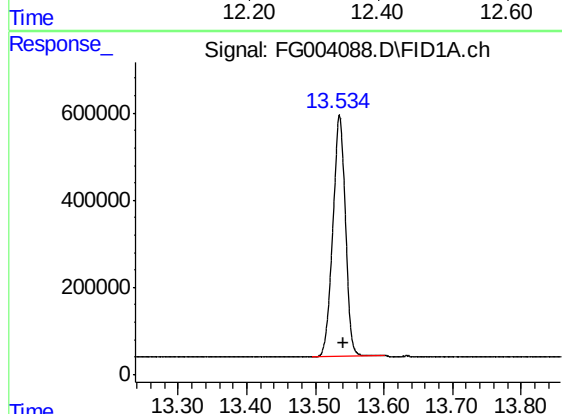


#8 N-DOCOSANE

R.T.: 13.535 min
Delta R.T.: -0.006 min
Response: 7061495
Conc: 49.75 ug/ml

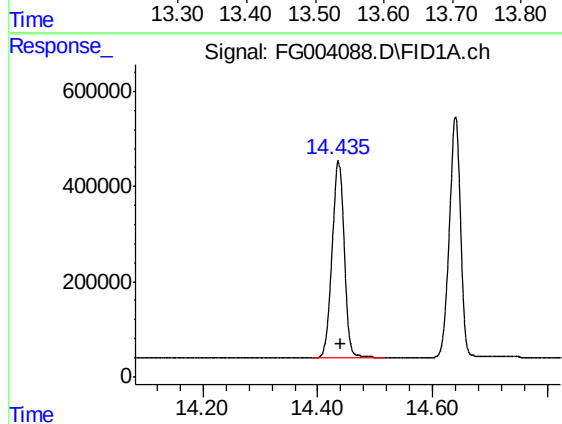


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.436 min
Delta R.T.: -0.005 min
Response: 6078951
Conc: 48.35 ug/ml

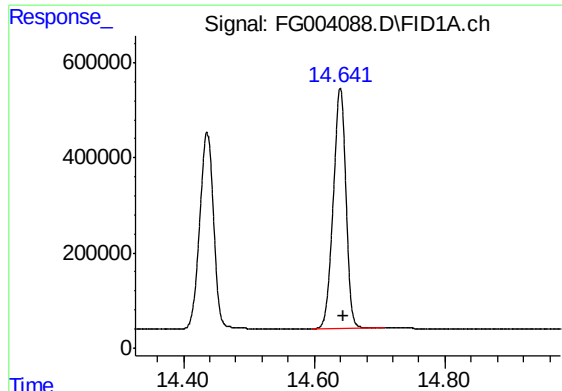


#10 N-TETRACOSANE

R.T.: 14.640 min
Delta R.T.: -0.004 min
Response: 6790871
Conc: 48.15 ug/ml

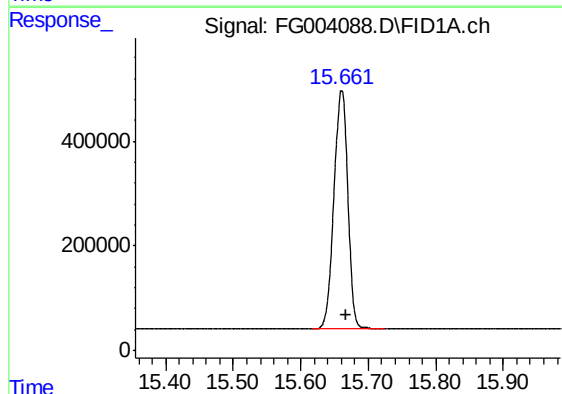

#11 N-HEXACOSANE

R.T.: 15.661 min
Delta R.T.: -0.006 min
Response: 6533758
Conc: 46.91 ug/ml

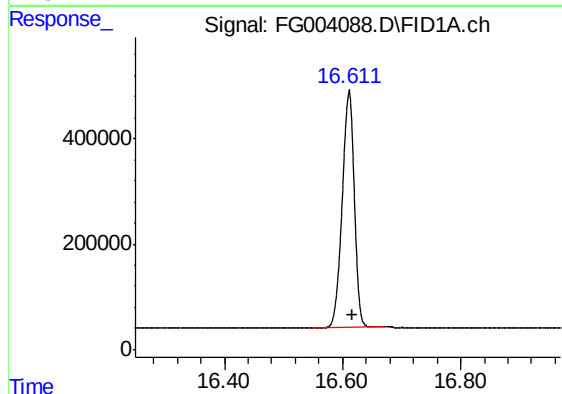

#12 N-OCTACOSANE

R.T.: 16.611 min
Delta R.T.: -0.006 min
Response: 6362267
Conc: 46.47 ug/ml