

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030819\
Data File : FG004100.D
Signal(s) : FID1A.ch
Acq On : 08 Mar 2019 15:08
Operator : AJ\SJ
Sample : K1787-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 08 22:33:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.435	1684800	13.401 ug/ml
Target Compounds			
4) N-TETRADECANE	8.044f	270193	1.938 ug/ml
14) N-DOTRIACONTANE	18.346	198984	1.573 ug/ml
16) N-HEXATRIACONTANE	19.903	367759	3.322 ug/ml
18) N-TETRACONTANE	21.444	408832	3.855 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030819\
Data File : FG004100.D
Signal(s) : FID1A.ch
Acq On : 08 Mar 2019 15:08
Operator : AJ\SJ
Sample : K1787-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 08 22:33:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

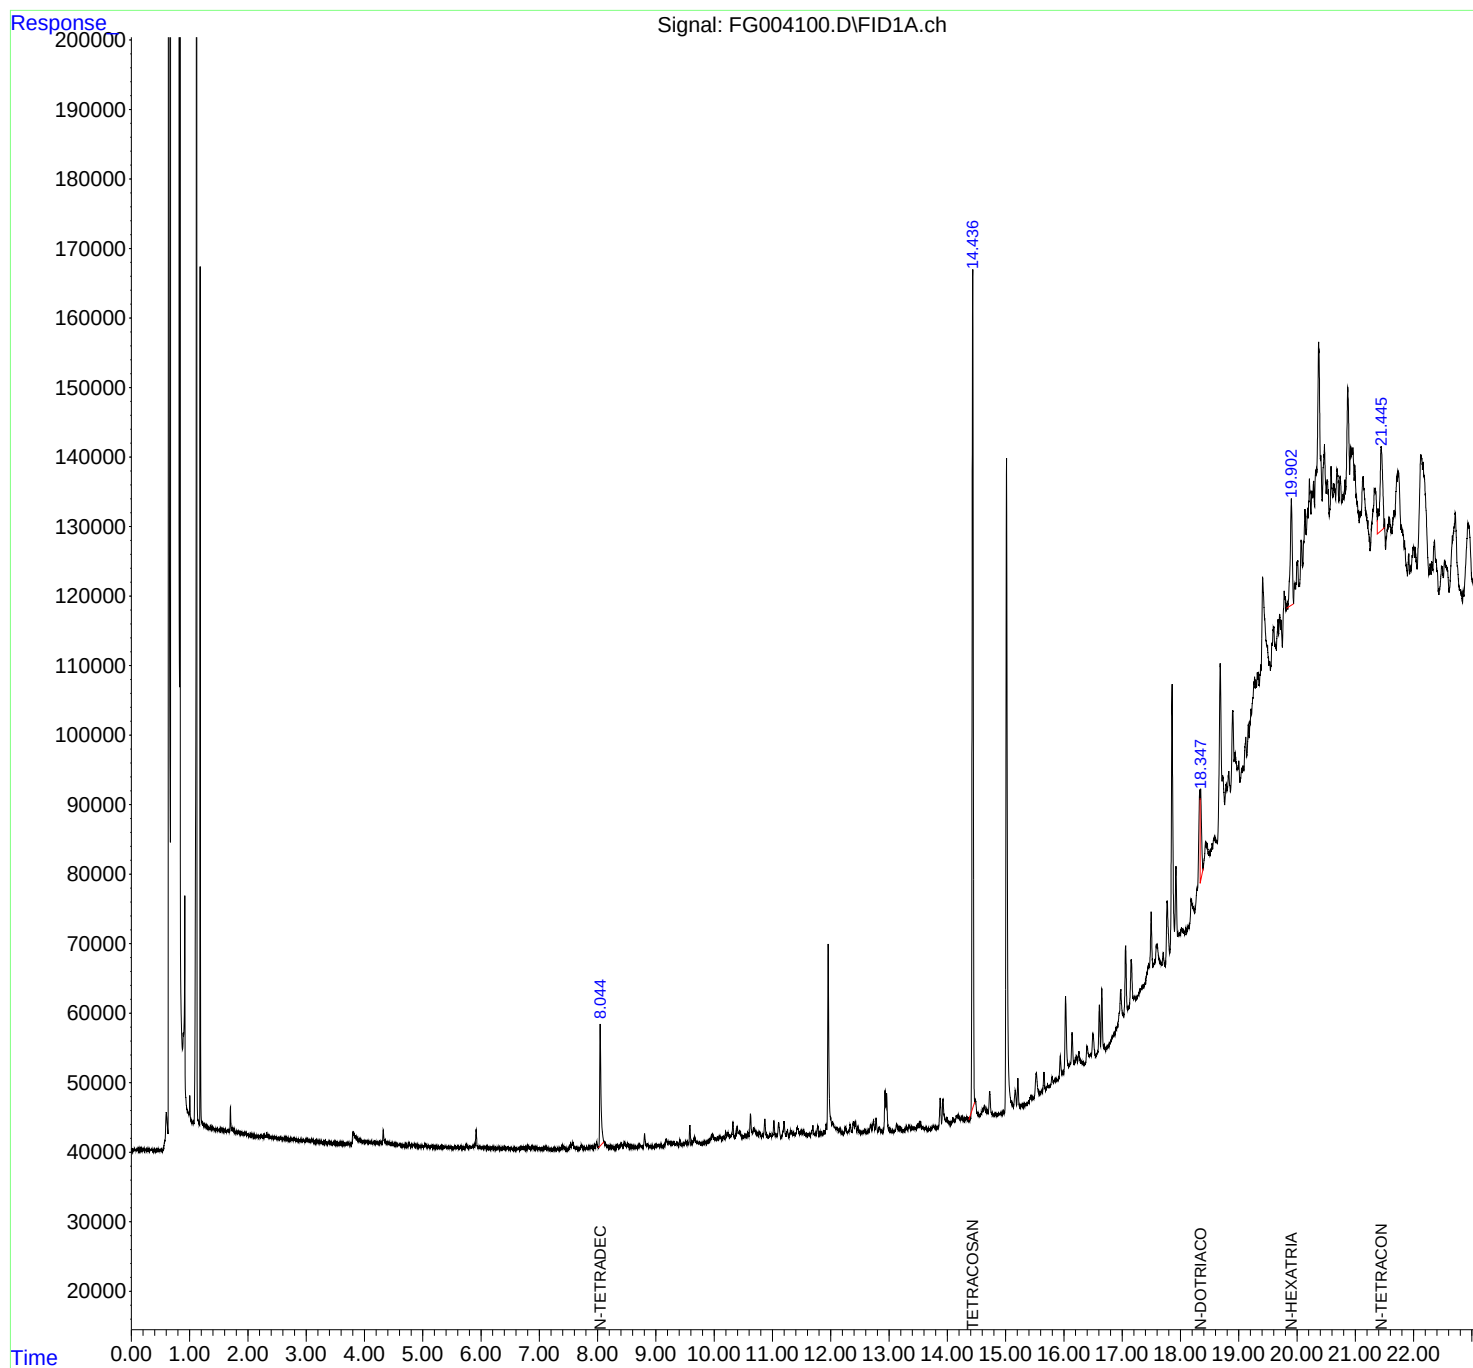

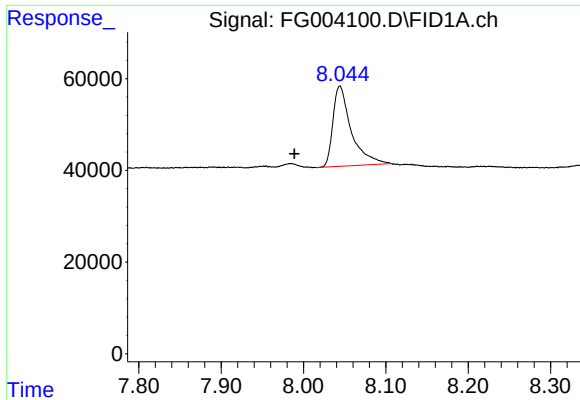


#4 N-TETRADECANE

R.T.: 8.044 min
Delta R.T.: 0.055 min
Response: 270193
Conc: 1.94 ug/ml

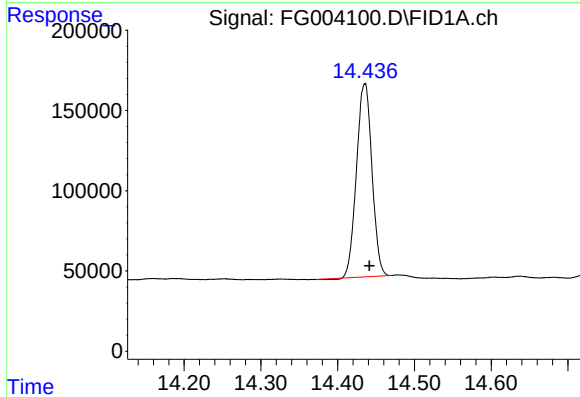


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.435 min
Delta R.T.: -0.006 min
Response: 1684800
Conc: 13.40 ug/ml

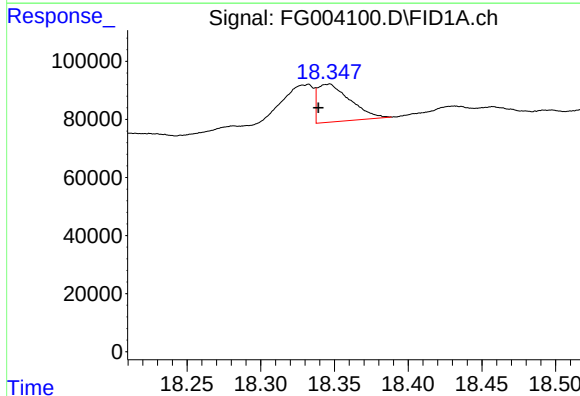


#14 N-DOTRIACONTANE

R.T.: 18.346 min
Delta R.T.: 0.007 min
Response: 198984
Conc: 1.57 ug/ml

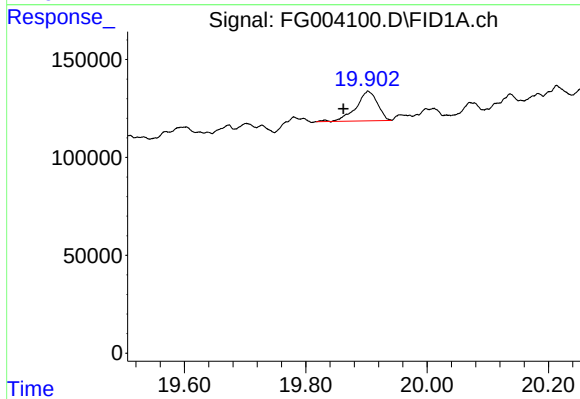

#16 N-HEXATRIACONTANE

R.T.: 19.903 min
Delta R.T.: 0.041 min
Response: 367759
Conc: 3.32 ug/ml

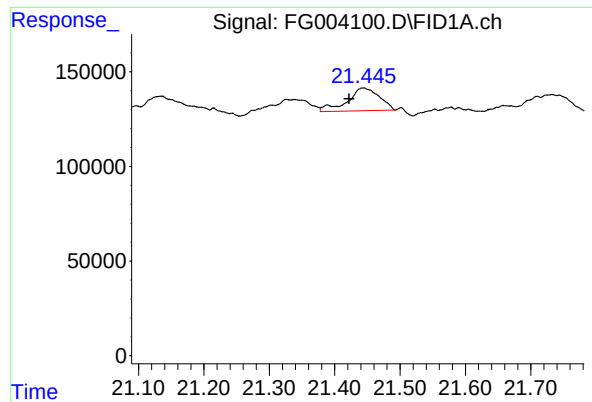

#18 N-TETRACONTANE

R.T.: 21.444 min
Delta R.T.: 0.022 min
Response: 408832
Conc: 3.85 ug/ml