

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG030823\  
 Data File : FG011546.D  
 Signal(s) : FID1A.ch  
 Acq On : 08 Mar 2023 20:42  
 Operator : YP\AJ  
 Sample : 01829-08 10X  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :  
 SS-08-20230306

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 03/09/2023  
 Supervised By :Ankita Jodhani 03/09/2023

Integration File: autoint1.e  
 Quant Time: Mar 08 23:32:51 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG022123.M  
 Quant Title :  
 QLast Update : Tue Feb 21 16:44:49 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.070 | 138935   | 1.321 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG030823\  
Data File : FG011546.D  
Signal(s) : FID1A.ch  
Acq On : 08 Mar 2023 20:42  
Operator : YP\AJ  
Sample : 01829-08 10X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
SS-08-20230306


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/09/2023  
Supervised By :Ankita Jodhani 03/09/2023

Integration File: autoint1.e  
Quant Time: Mar 08 23:32:51 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG022123.M  
Quant Title :  
QLast Update : Tue Feb 21 16:44:49 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

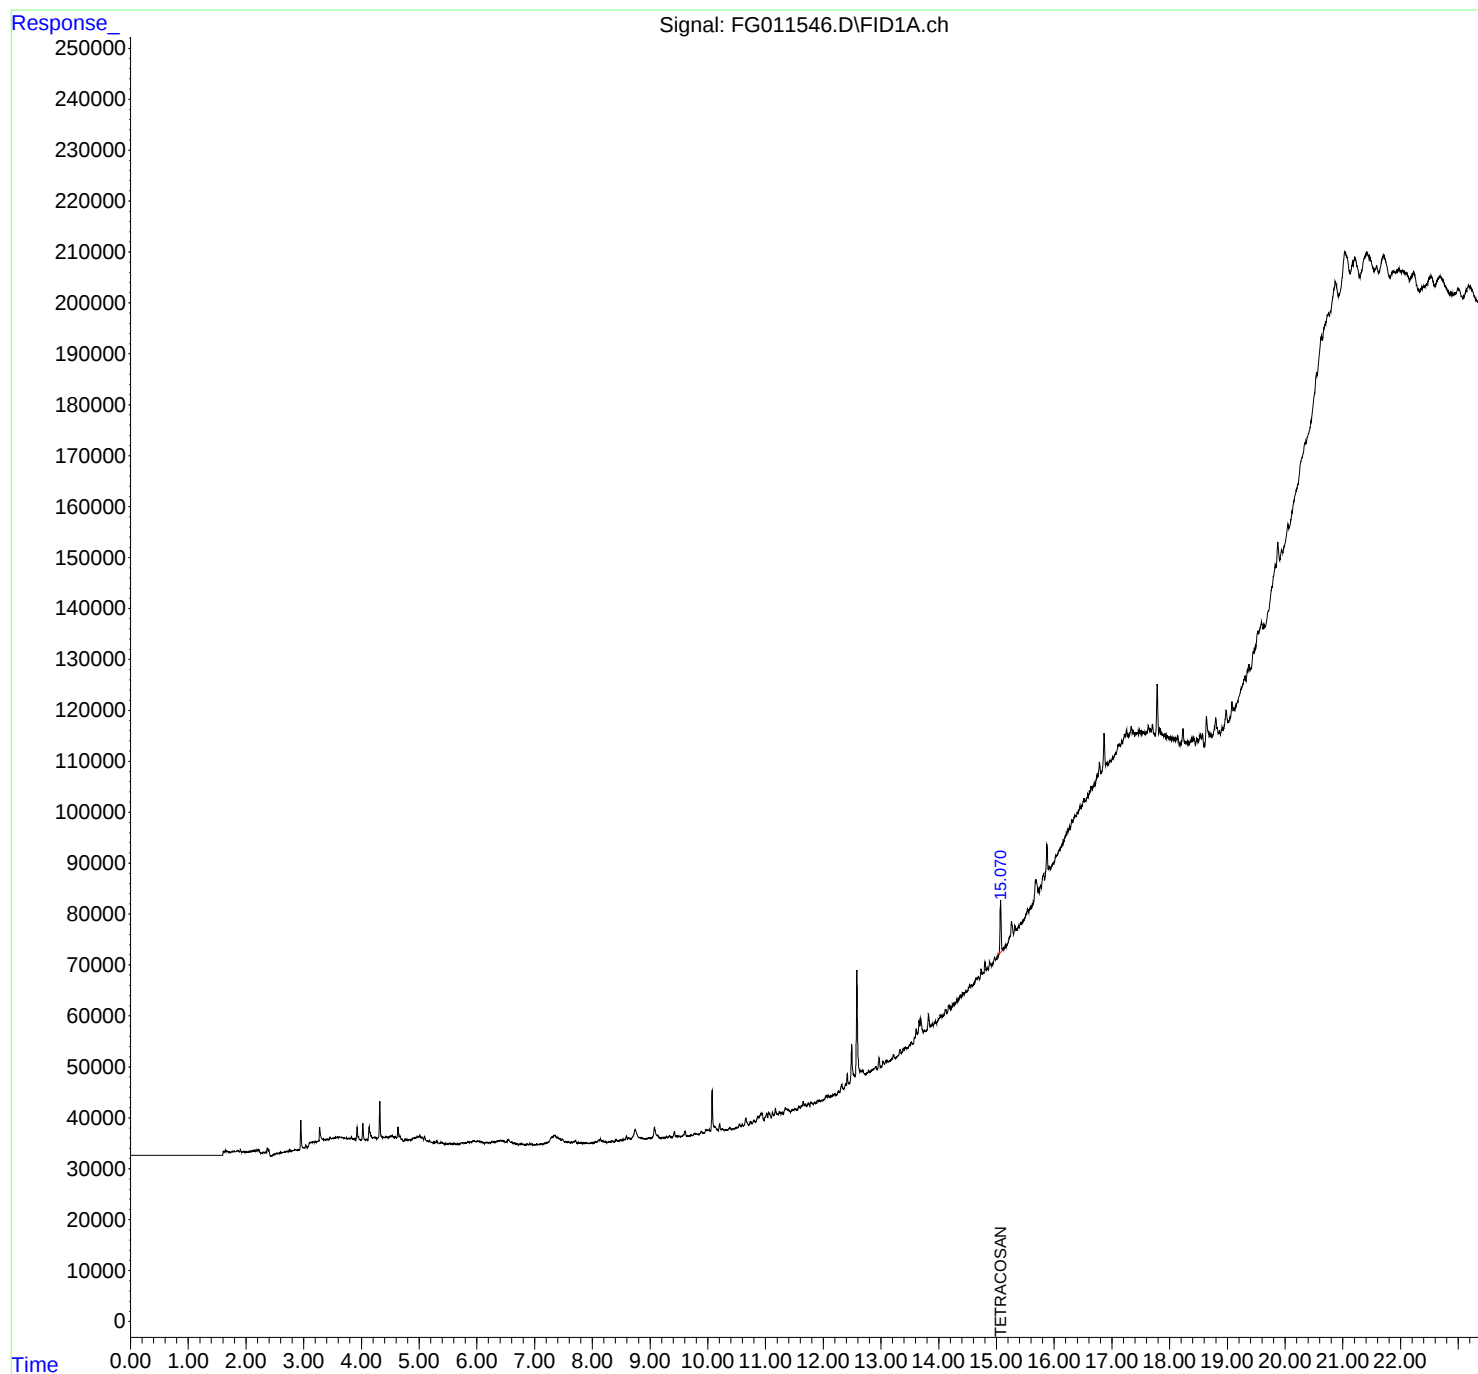

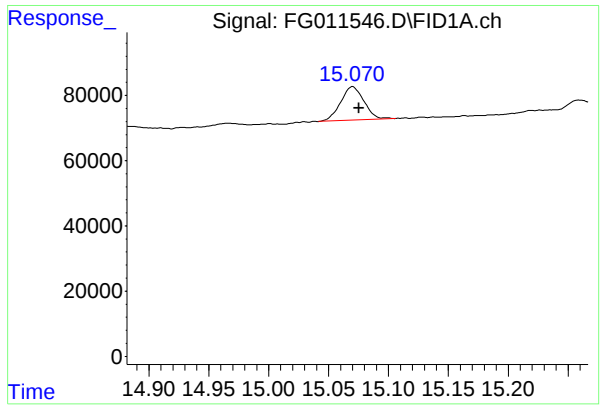

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.070 min  
Delta R.T.: -0.006 min  
Response: 138935  
Conc: 1.32 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
SS-08-20230306

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/09/2023  
Supervised By :Ankita Jodhani 03/09/2023