

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
Data File : FG007662.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2021 14:32
Operator : DD\AJ
Sample : M1603-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 02:04:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.455	1749832	13.123 ug/ml
Target Compounds			
4) N-TETRADECANE	8.045f	123572	0.766 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
Data File : FG007662.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2021 14:32
Operator : DD\AJ
Sample : M1603-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 02:04:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

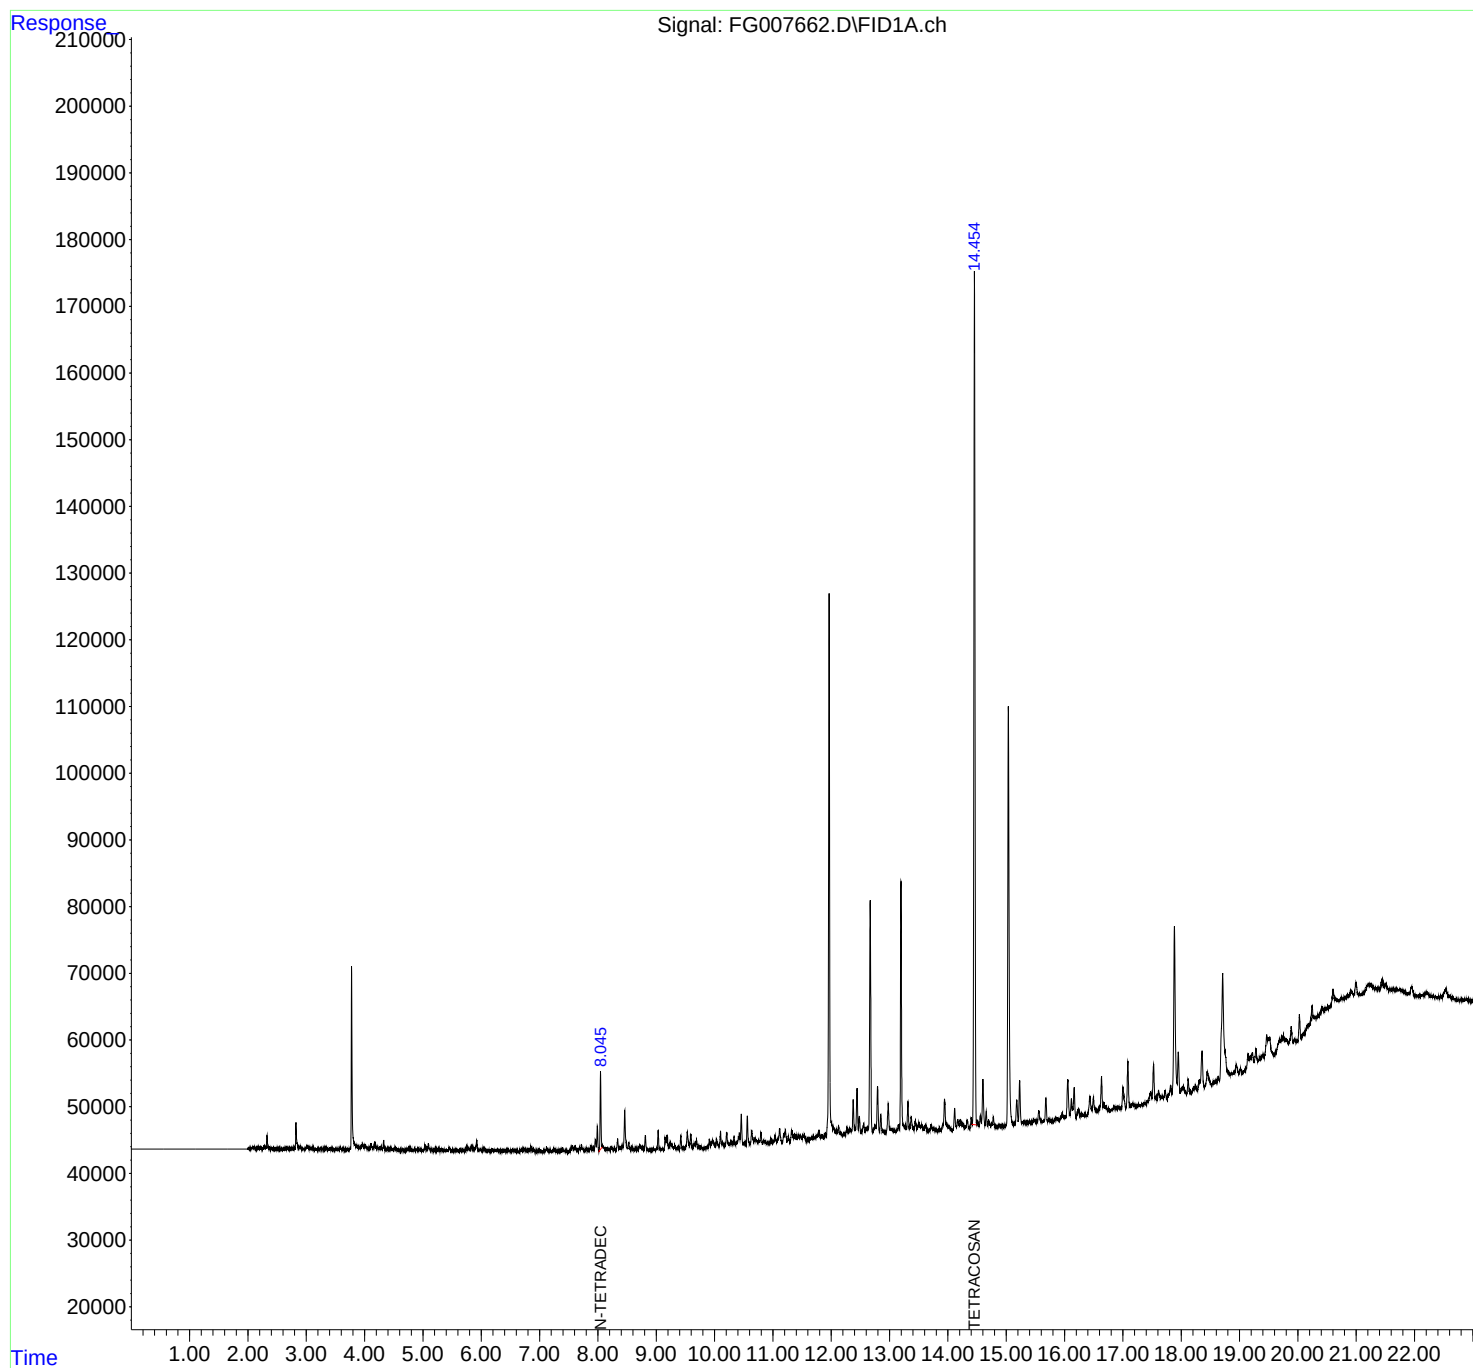


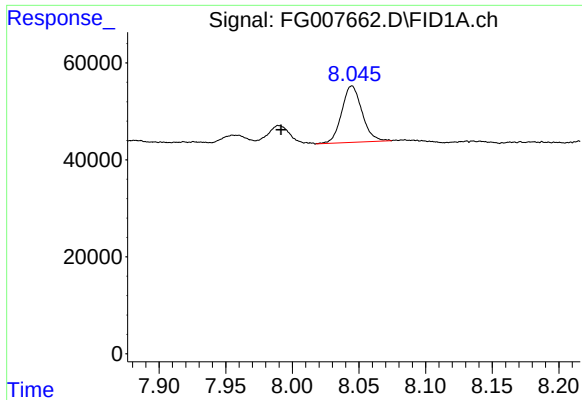

#4 N-TETRADECANE

R.T.: 8.045 min
Delta R.T.: 0.053 min
Response: 123572
Conc: 0.77 ug/ml

Instrument :
FID_G
ClientSampleId :

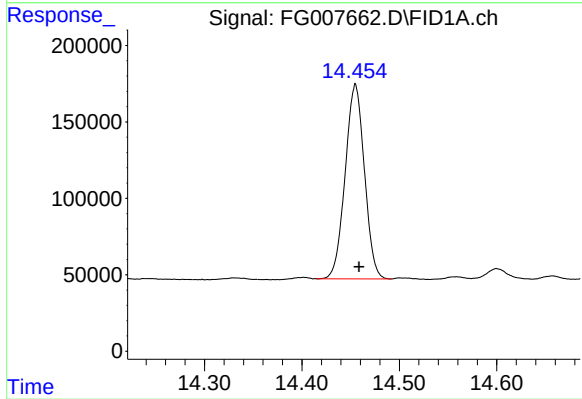

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.455 min
Delta R.T.: -0.004 min
Response: 1749832
Conc: 13.12 ug/ml