

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
 Data File : FG007657.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2021 10:48
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Mar 10 02:03:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
 Quant Title :
 QLast Update : Fri Mar 05 08:57:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	6118461	45.887 ug/ml
Target Compounds			
2) N-DECANE	4.177	7859116	50.286 ug/ml
3) N-DODECANE	6.197	7875668	49.937 ug/ml
4) N-TETRADECANE	7.994	7937447	49.207 ug/ml
5) N-HEXADECANE	9.598	7741875	48.254 ug/ml
6) N-OCTADECANE	11.042	7617417	47.331 ug/ml
7) N-EICOSANE	12.355	7359091	46.584 ug/ml
8) N-DOCOSANE	13.556	7108938	46.061 ug/ml
10) N-TETRACOSANE	14.663	6882654	45.664 ug/ml
11) N-HEXACOSANE	15.687	6604686	45.536 ug/ml
12) N-OCTACOSANE	16.639	6461551	46.067 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
Data File : FG007657.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2021 10:48
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Mar 10 02:03:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

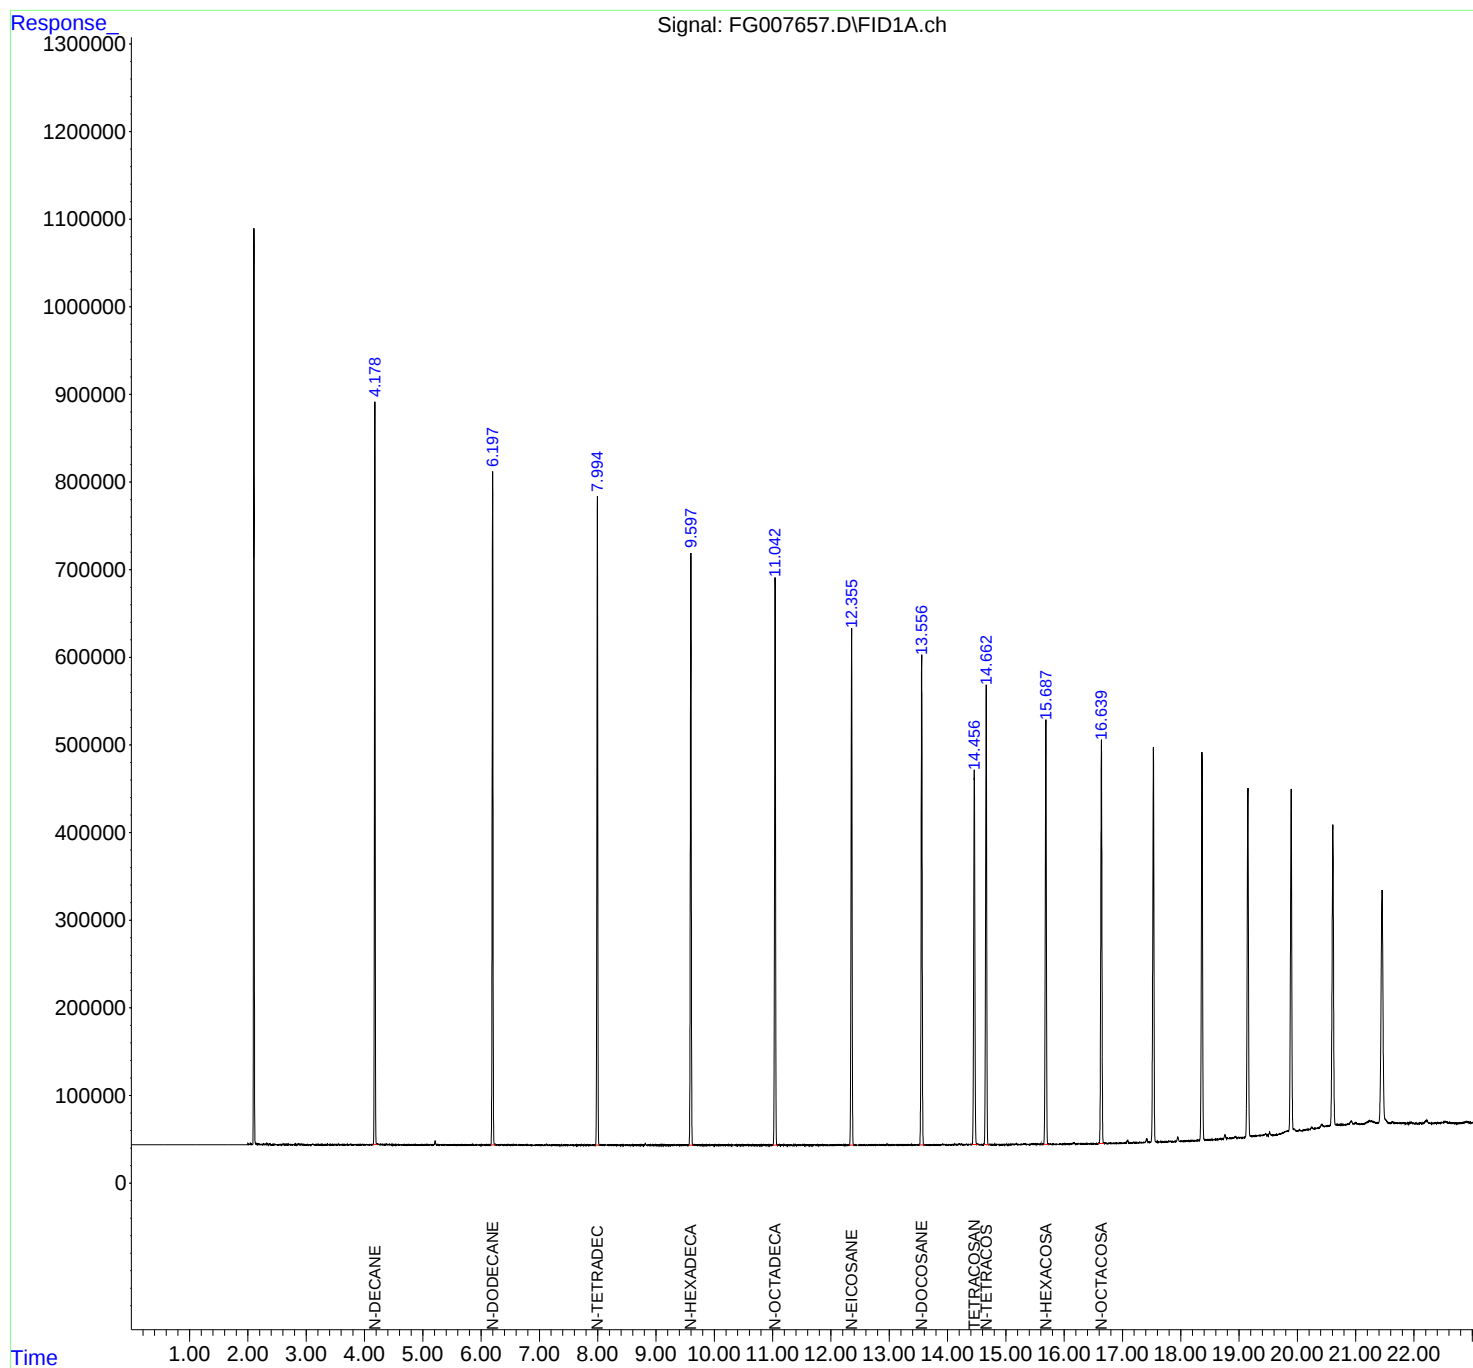


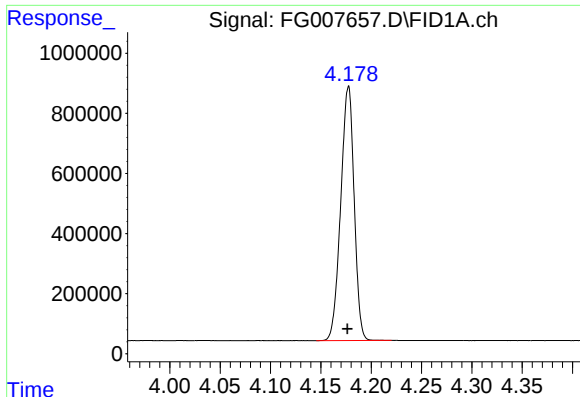

#2 N-DECANE


R.T.: 4.177 min
Delta R.T.: 0.001 min
Response: 7859116
Conc: 50.29 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

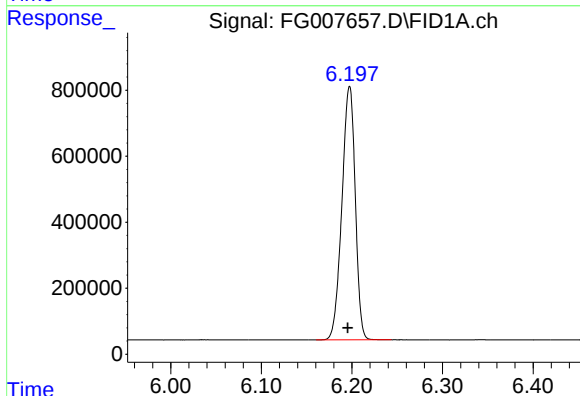


#3 N-DODECANE

R.T.: 6.197 min
Delta R.T.: 0.002 min
Response: 7875668
Conc: 49.94 ug/ml

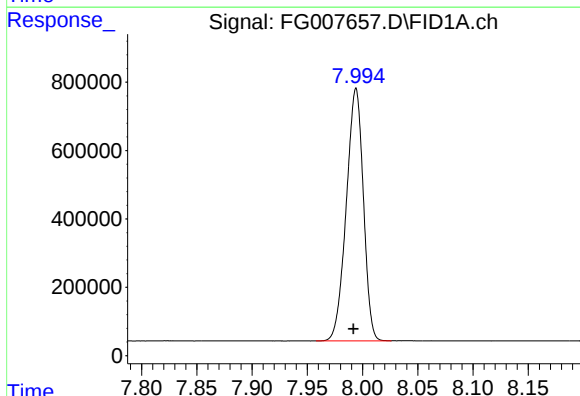


#4 N-TETRADECANE

R.T.: 7.994 min
Delta R.T.: 0.002 min
Response: 7937447
Conc: 49.21 ug/ml

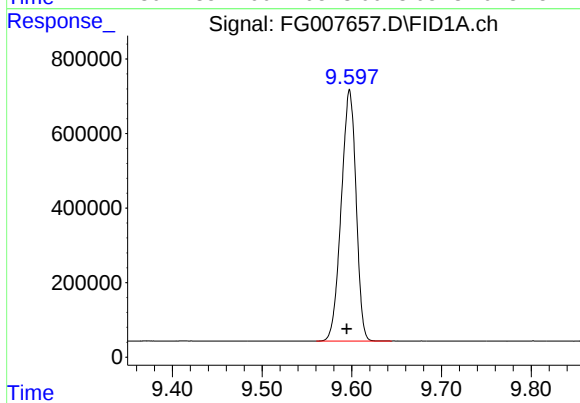

#5 N-HEXADECANE


R.T.: 9.598 min
Delta R.T.: 0.003 min
Response: 7741875
Conc: 48.25 ug/ml

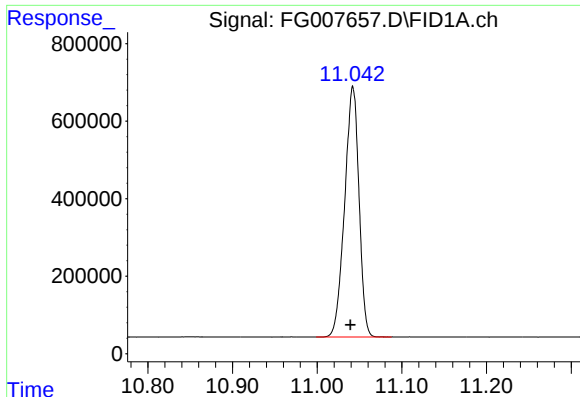

#6 N-OCTADECANE


R.T.: 11.042 min
Delta R.T.: 0.003 min
Response: 7617417
Conc: 47.33 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

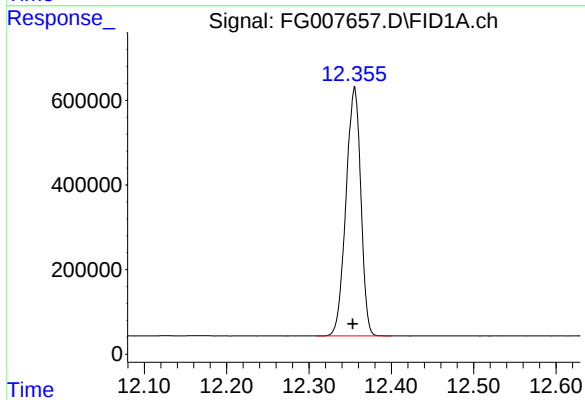


#7 N-EICOSANE

R.T.: 12.355 min
Delta R.T.: 0.002 min
Response: 7359091
Conc: 46.58 ug/ml

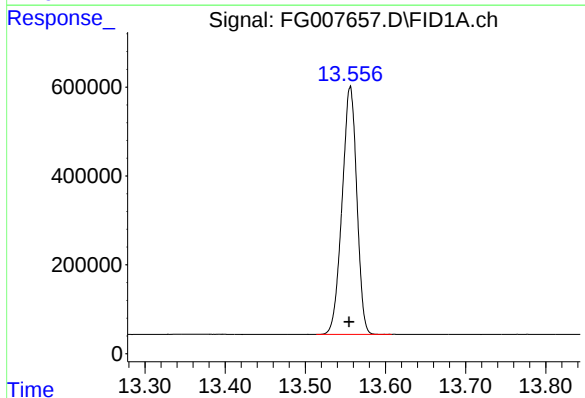


#8 N-DOCOSANE

R.T.: 13.556 min
Delta R.T.: 0.002 min
Response: 7108938
Conc: 46.06 ug/ml

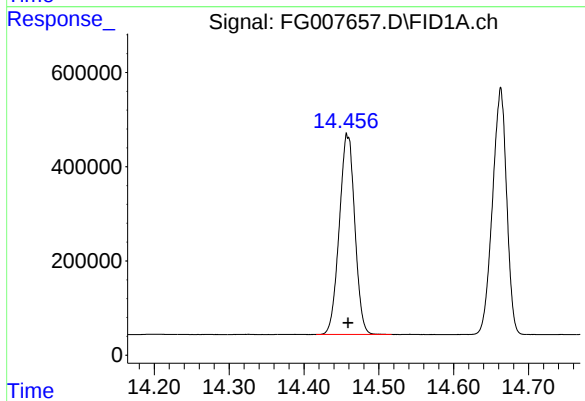

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.458 min
Delta R.T.: 0.000 min
Response: 6118461
Conc: 45.89 ug/ml

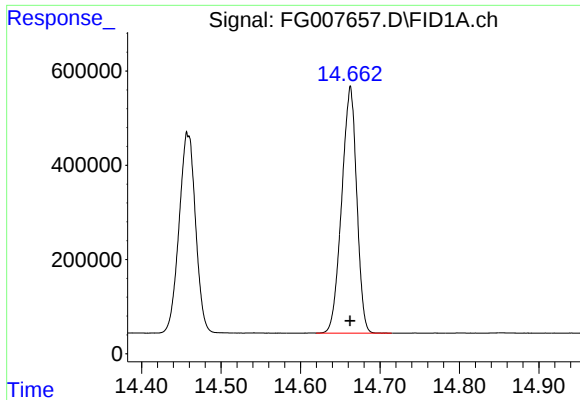

#10 N-TETRACOSANE


R.T.: 14.663 min
Delta R.T.: 0.000 min
Response: 6882654
Conc: 45.66 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

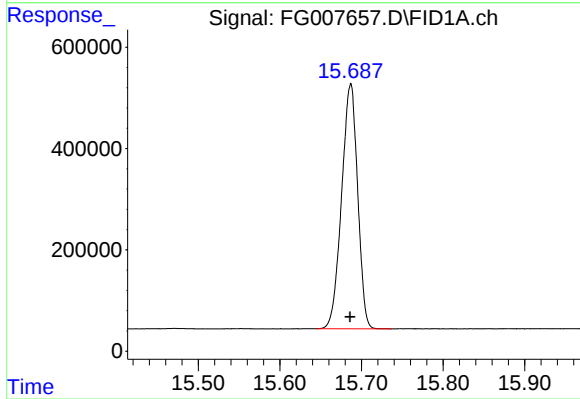

#11 N-HEXACOSANE

R.T.: 15.687 min
Delta R.T.: 0.000 min
Response: 6604686
Conc: 45.54 ug/ml

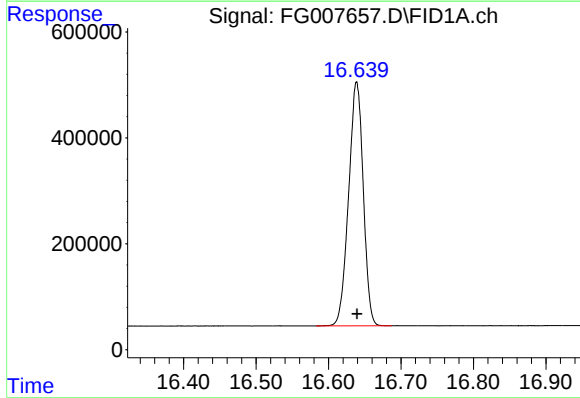

#12 N-OCTACOSANE

R.T.: 16.639 min
Delta R.T.: 0.000 min
Response: 6461551
Conc: 46.07 ug/ml