

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
 Data File : FG007664.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2021 15:35
 Operator : DD\AJ
 Sample : M1603-01MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 31-NORTHMSD

Integration File: autoint1.e
 Quant Time: Mar 10 02:05:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
 Quant Title :
 QLast Update : Fri Mar 05 08:57:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.454	1875494	14.066 ug/ml
Target Compounds			
2) N-DECANE	4.176	2760379	17.662 ug/ml
3) N-DODECANE	6.195	2889881	18.324 ug/ml
4) N-TETRADECANE	7.991	3057393	18.954 ug/ml
5) N-HEXADECANE	9.594	3018168	18.812 ug/ml
6) N-OCTADECANE	11.039	2976086	18.492 ug/ml
7) N-EICOSANE	12.351	2986609	18.906 ug/ml
8) N-DOCOSANE	13.553	2822633	18.289 ug/ml
10) N-TETRACOSANE	14.659	2712444	17.996 ug/ml
11) N-HEXACOSANE	15.682	2659996	18.339 ug/ml
12) N-OCTACOSANE	16.635	2640370	18.824 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
Data File : FG007664.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2021 15:35
Operator : DD\AJ
Sample : M1603-01MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
31-NORTHMSD

Integration File: autoint1.e
Quant Time: Mar 10 02:05:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

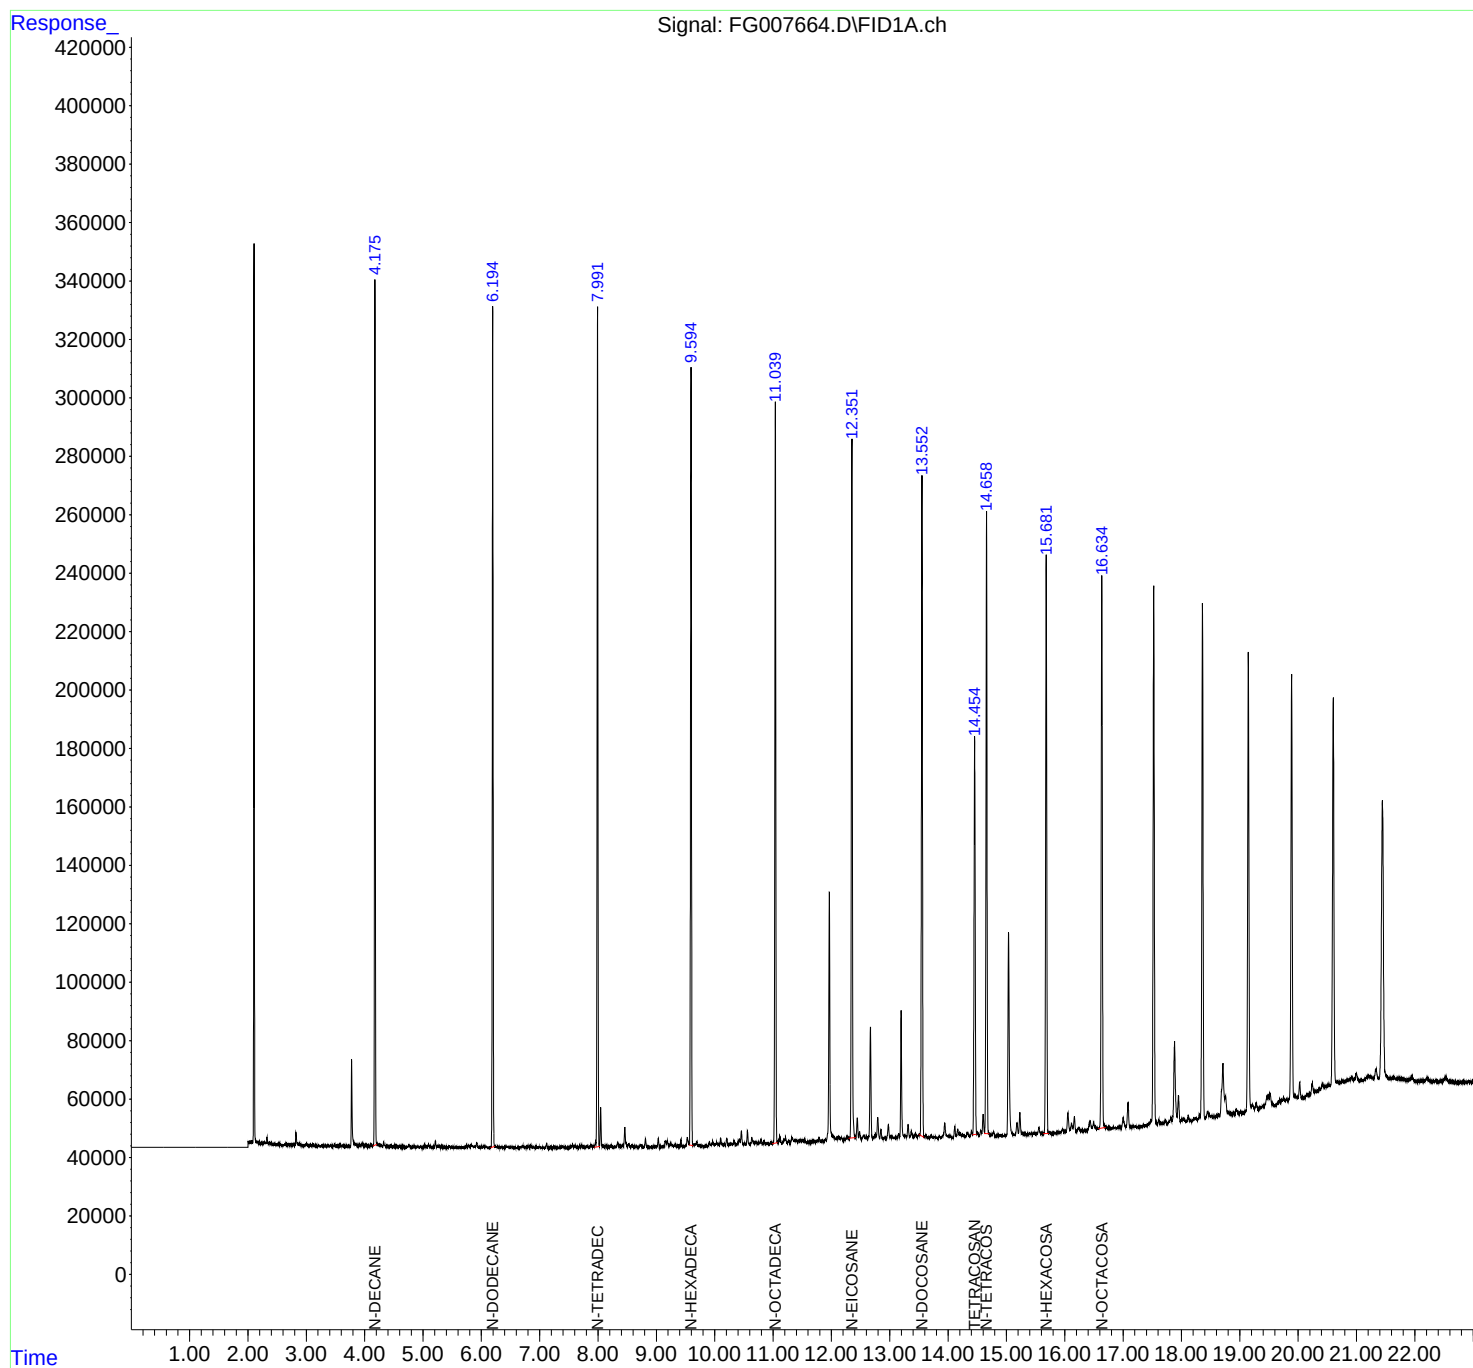


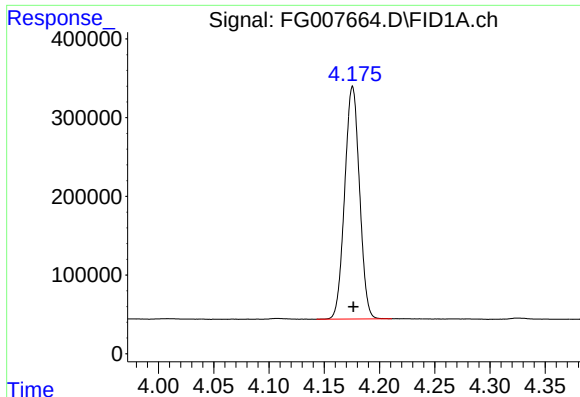

#2 N-DECANE


R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 2760379
Conc: 17.66 ug/ml

Instrument :
FID_G
ClientSampleId :
31-NORTHMSD

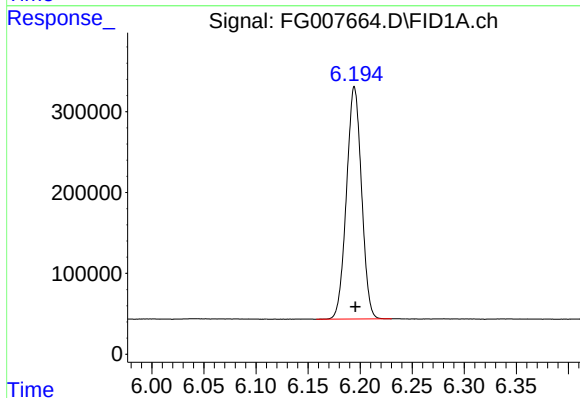


#3 N-DODECANE

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 2889881
Conc: 18.32 ug/ml

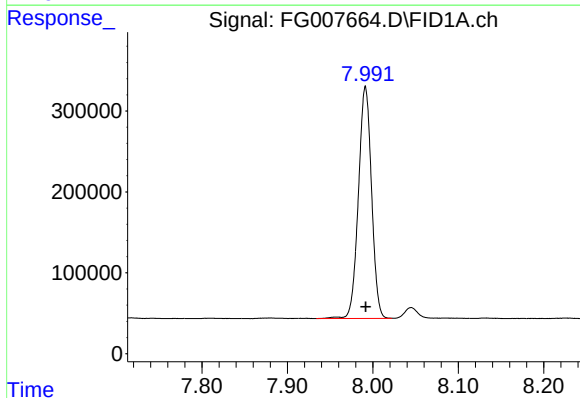


#4 N-TETRADECANE

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 3057393
Conc: 18.95 ug/ml

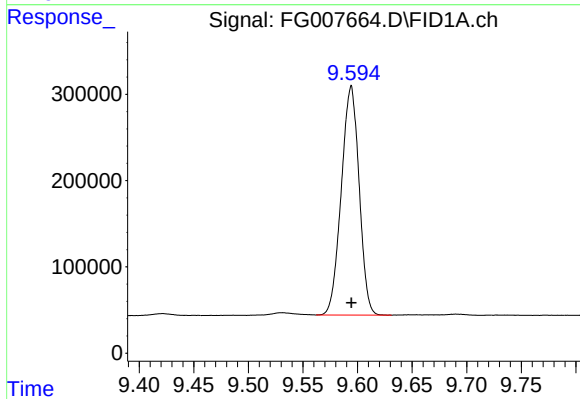

#5 N-HEXADECANE


R.T.: 9.594 min
Delta R.T.: 0.000 min
Response: 3018168
Conc: 18.81 ug/ml

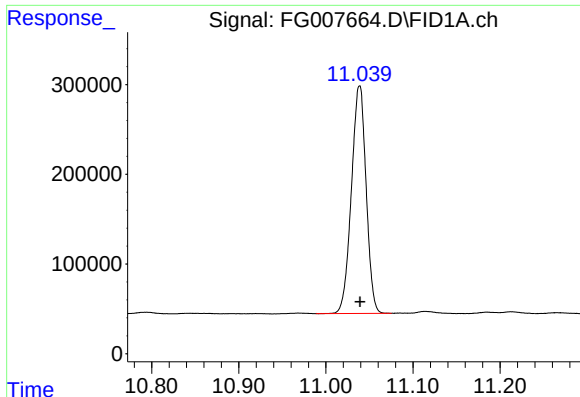

#6 N-OCTADECANE


R.T.: 11.039 min
Delta R.T.: 0.000 min
Response: 2976086
Conc: 18.49 ug/ml

Instrument :
FID_G
ClientSampleId :
31-NORTHMSD

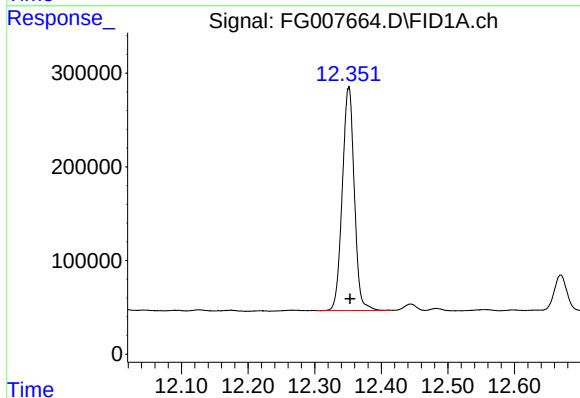


#7 N-EICOSANE

R.T.: 12.351 min
Delta R.T.: -0.002 min
Response: 2986609
Conc: 18.91 ug/ml

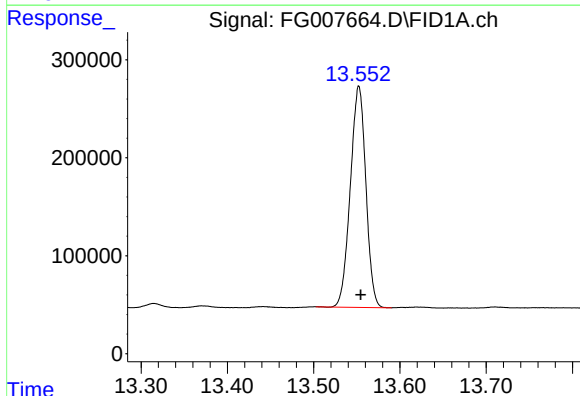


#8 N-DOCOSANE

R.T.: 13.553 min
Delta R.T.: -0.002 min
Response: 2822633
Conc: 18.29 ug/ml

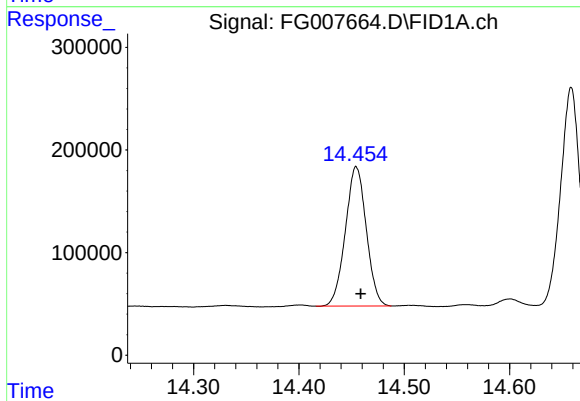

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.454 min
Delta R.T.: -0.004 min
Response: 1875494
Conc: 14.07 ug/ml

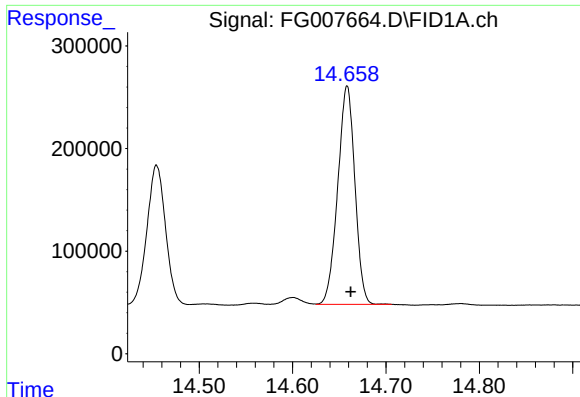

#10 N-TETRACOSANE


R.T.: 14.659 min
Delta R.T.: -0.004 min
Response: 2712444
Conc: 18.00 ug/ml

Instrument :
FID_G
ClientSampleId :
31-NORTHMSD

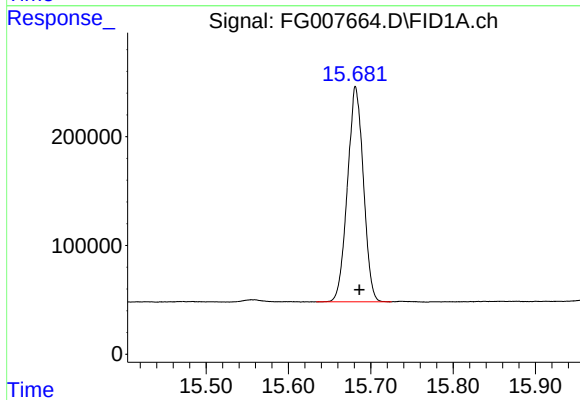

#11 N-HEXACOSANE

R.T.: 15.682 min
Delta R.T.: -0.005 min
Response: 2659996
Conc: 18.34 ug/ml

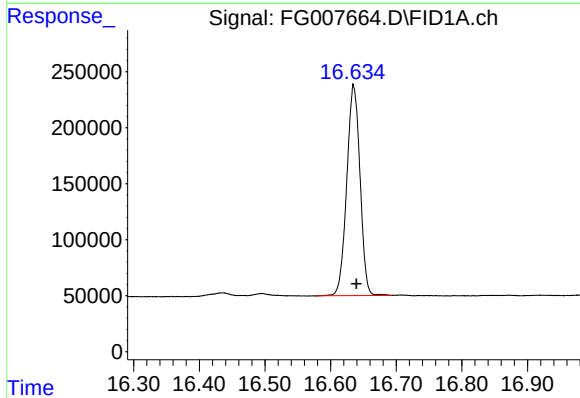

#12 N-OCTACOSANE

R.T.: 16.635 min
Delta R.T.: -0.004 min
Response: 2640370
Conc: 18.82 ug/ml