

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
Data File : FG007667.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2021 17:11
Operator : DD\AJ
Sample : M1597-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-030821

Manual Integrations
APPROVED

Ankita
3/10/2021 10:15:15 AM

Integration File: autoint1.e
Quant Time: Mar 10 02:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	170392	1.278 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030921\
Data File : FG007667.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2021 17:11
Operator : DD\AJ
Sample : M1597-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
AU-06-030821


Manual Integrations
APPROVED

Ankita
3/10/2021 10:15:15 AM

Integration File: autoint1.e
Quant Time: Mar 10 02:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

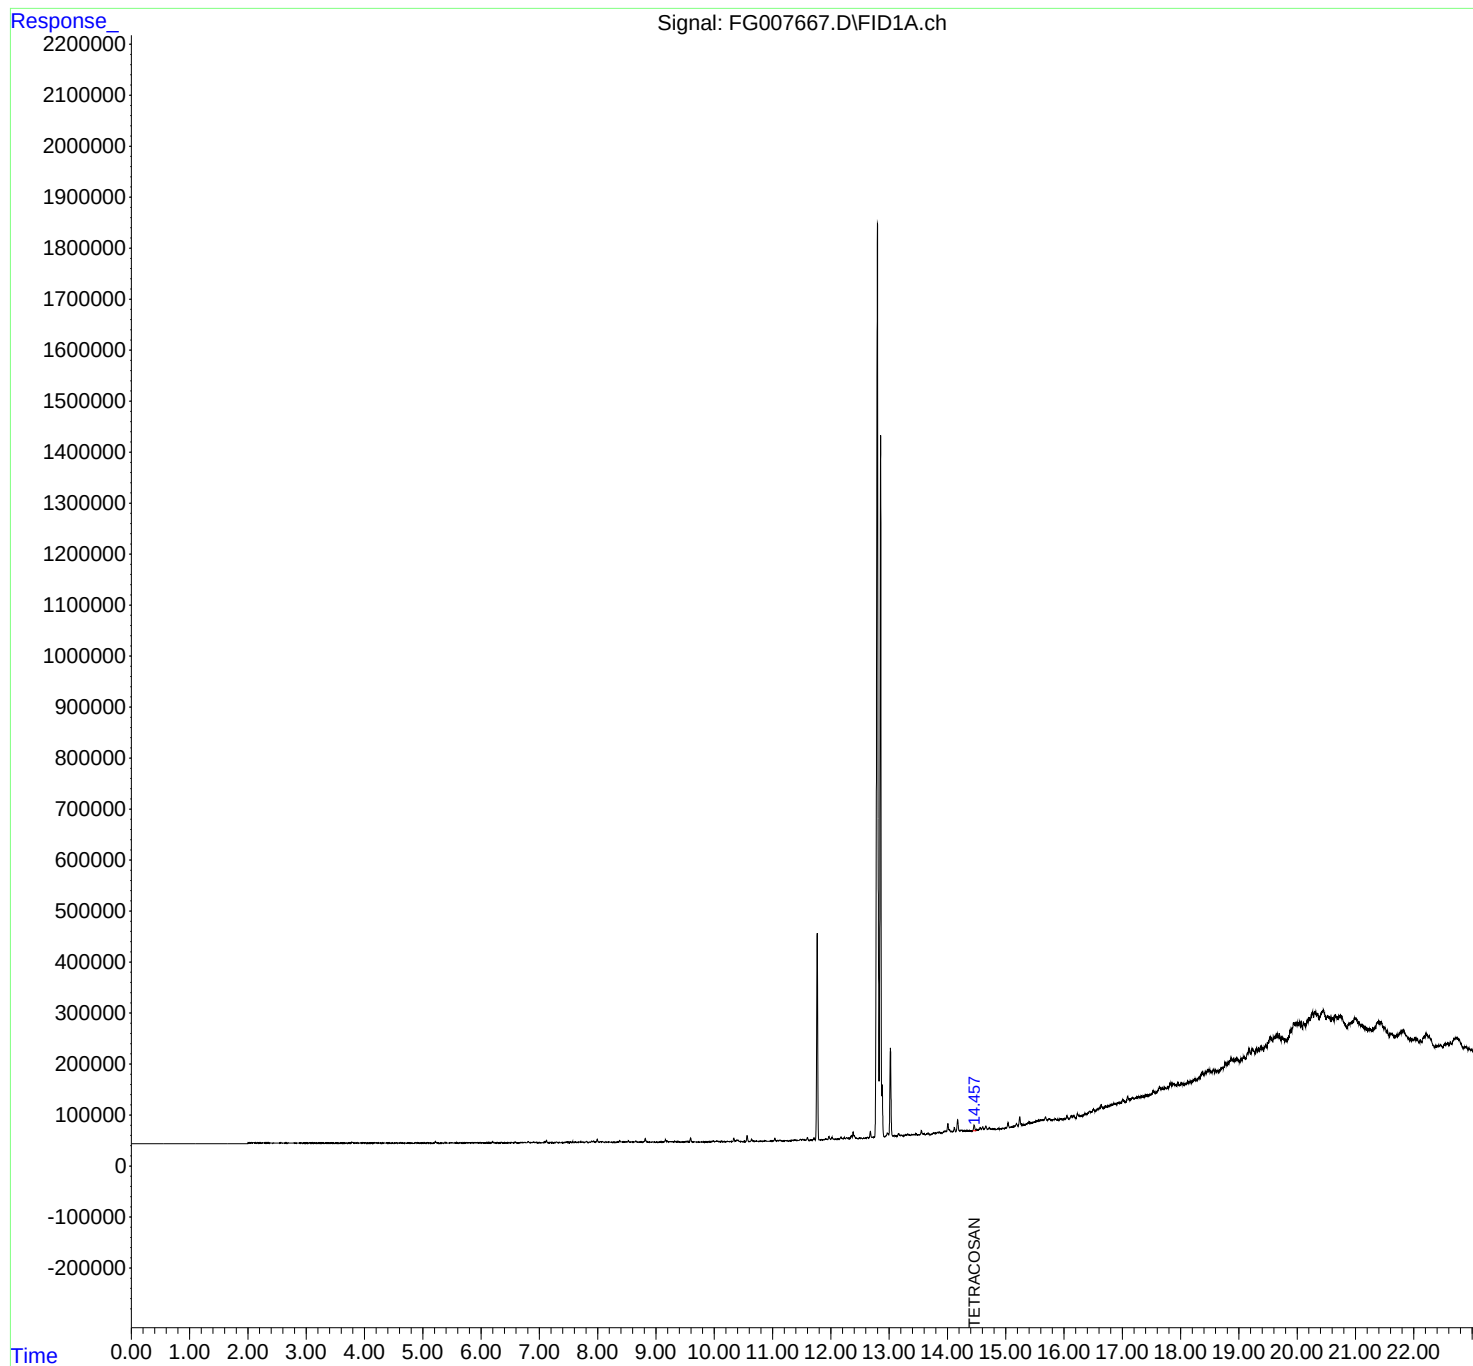

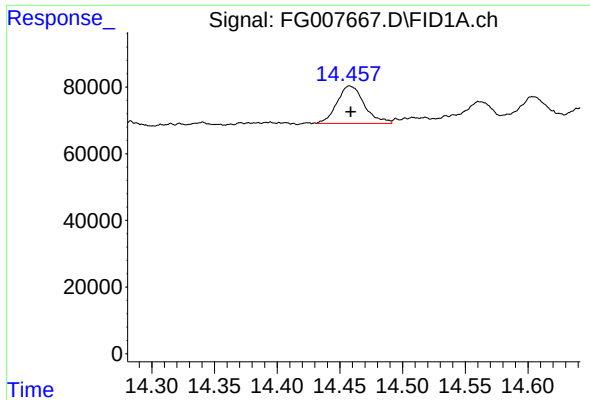

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: -0.002 min
Response: 170392
Conc: 1.28 ug/ml m

Instrument :
FID_G
ClientSampleId :
AU-06-030821

Manual Integrations
APPROVED

Ankita
3/10/2021 10:15:15 AM