

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030923\
Data File : FG011557.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2023 10:54
Operator : YP\AJ
Sample : 01829-06 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 14:04:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.969	7133	0.071 ug/ml
15)	N-TETRATRIACONTANE	19.817	7128	0.076 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030923\
Data File : FG011557.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2023 10:54
Operator : YP\AJ
Sample : 01829-06 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 14:04:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

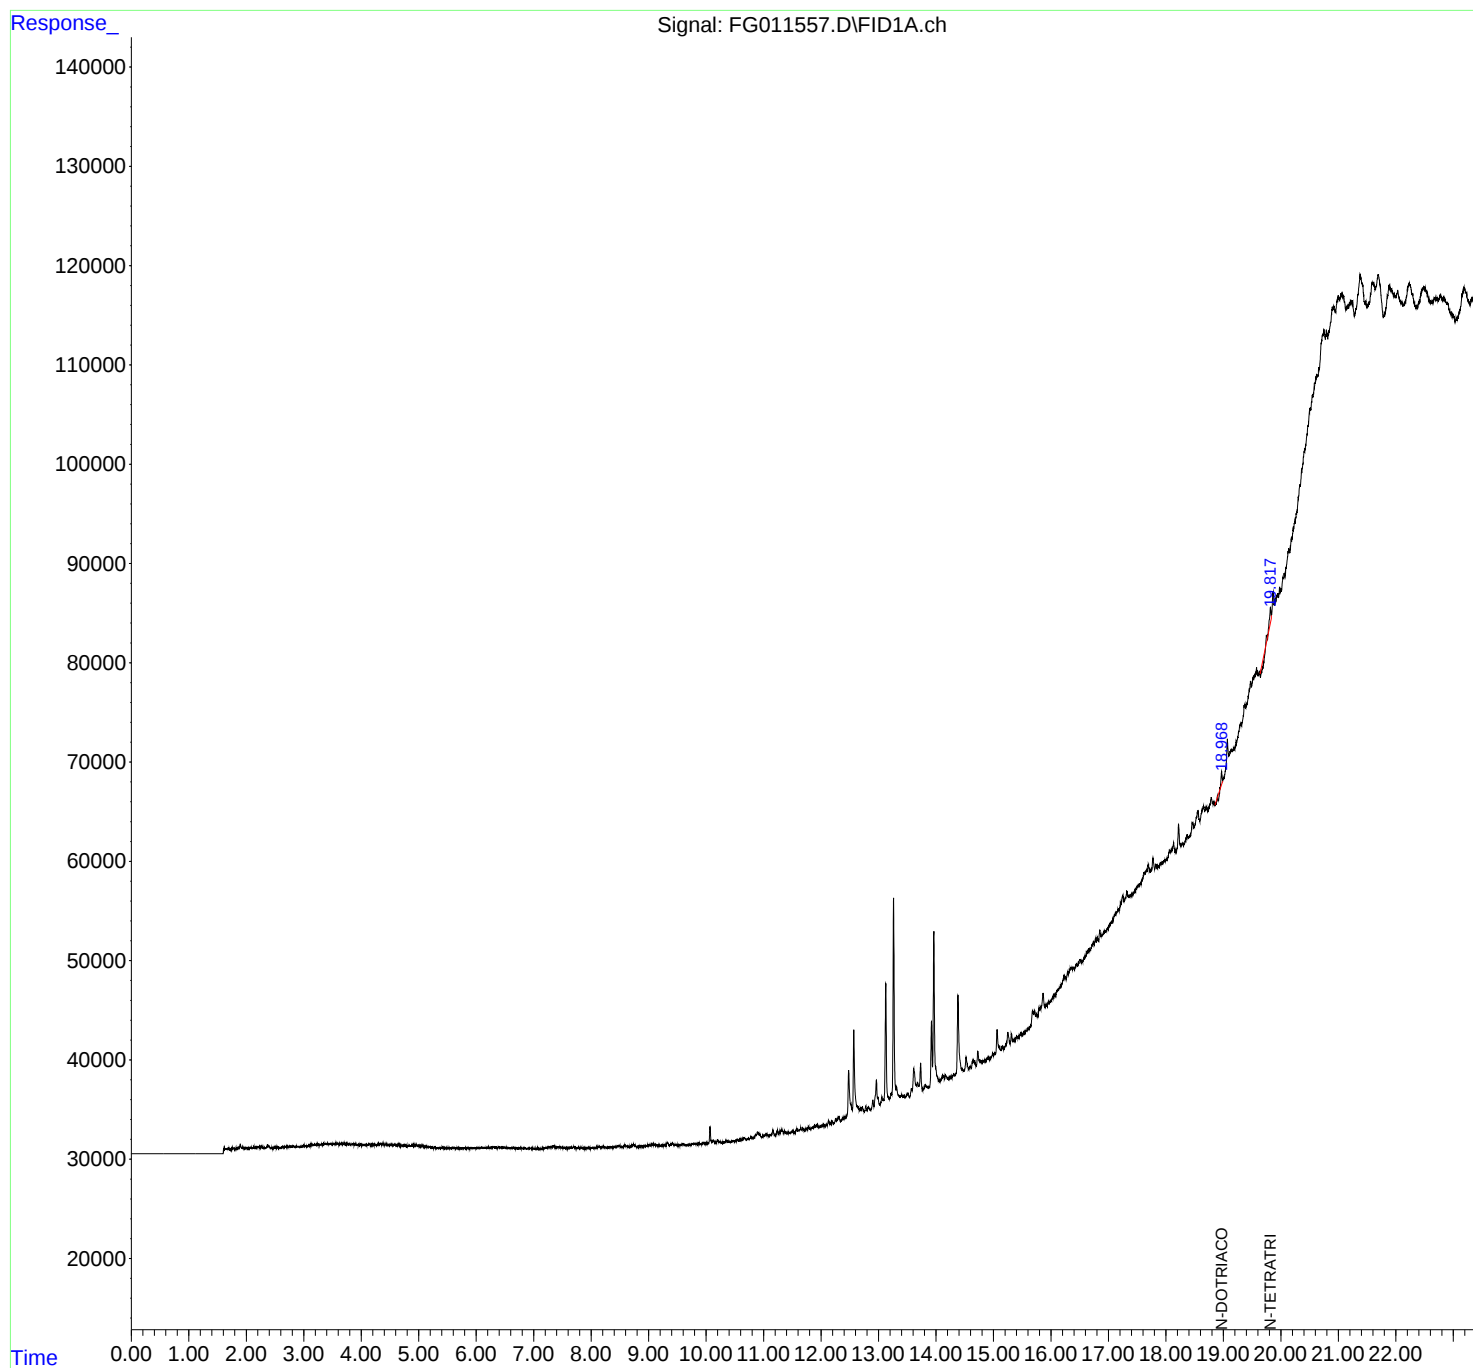


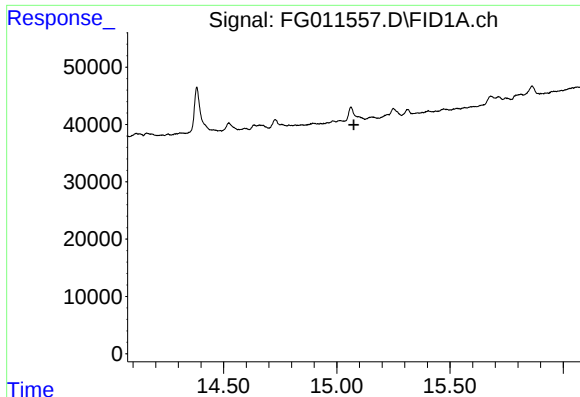

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.075 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

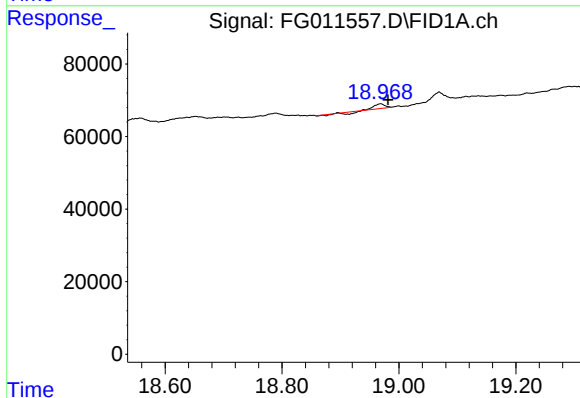

#14 N-DOTRIACONTANE

R.T.: 18.969 min
Delta R.T.: -0.013 min
Response: 7133
Conc: 0.07 ug/ml

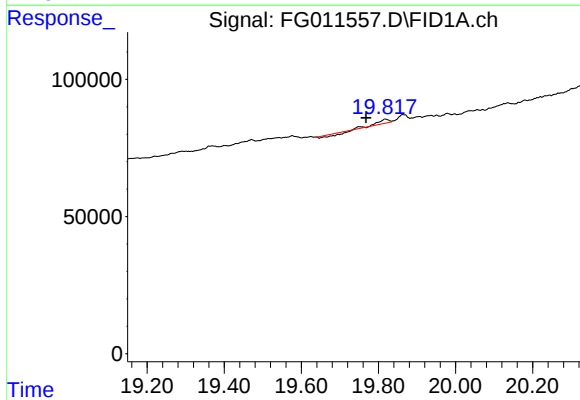

#15 N-TETRATRIACONTANE

R.T.: 19.817 min
Delta R.T.: 0.050 min
Response: 7128
Conc: 0.08 ug/ml