

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030923\
 Data File : FG011557.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2023 10:54
 Operator : YP\AJ
 Sample : 01829-06 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SS-06-20230306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/09/2023
 Supervised By :Ankita Jodhani 03/10/2023

Integration File: autoint1.e
 Quant Time: Mar 09 14:04:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:44:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.062	44220	0.420 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030923\
Data File : FG011557.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2023 10:54
Operator : YP\AJ
Sample : 01829-06 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
SS-06-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/10/2023

Integration File: autoint1.e
Quant Time: Mar 09 14:04:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

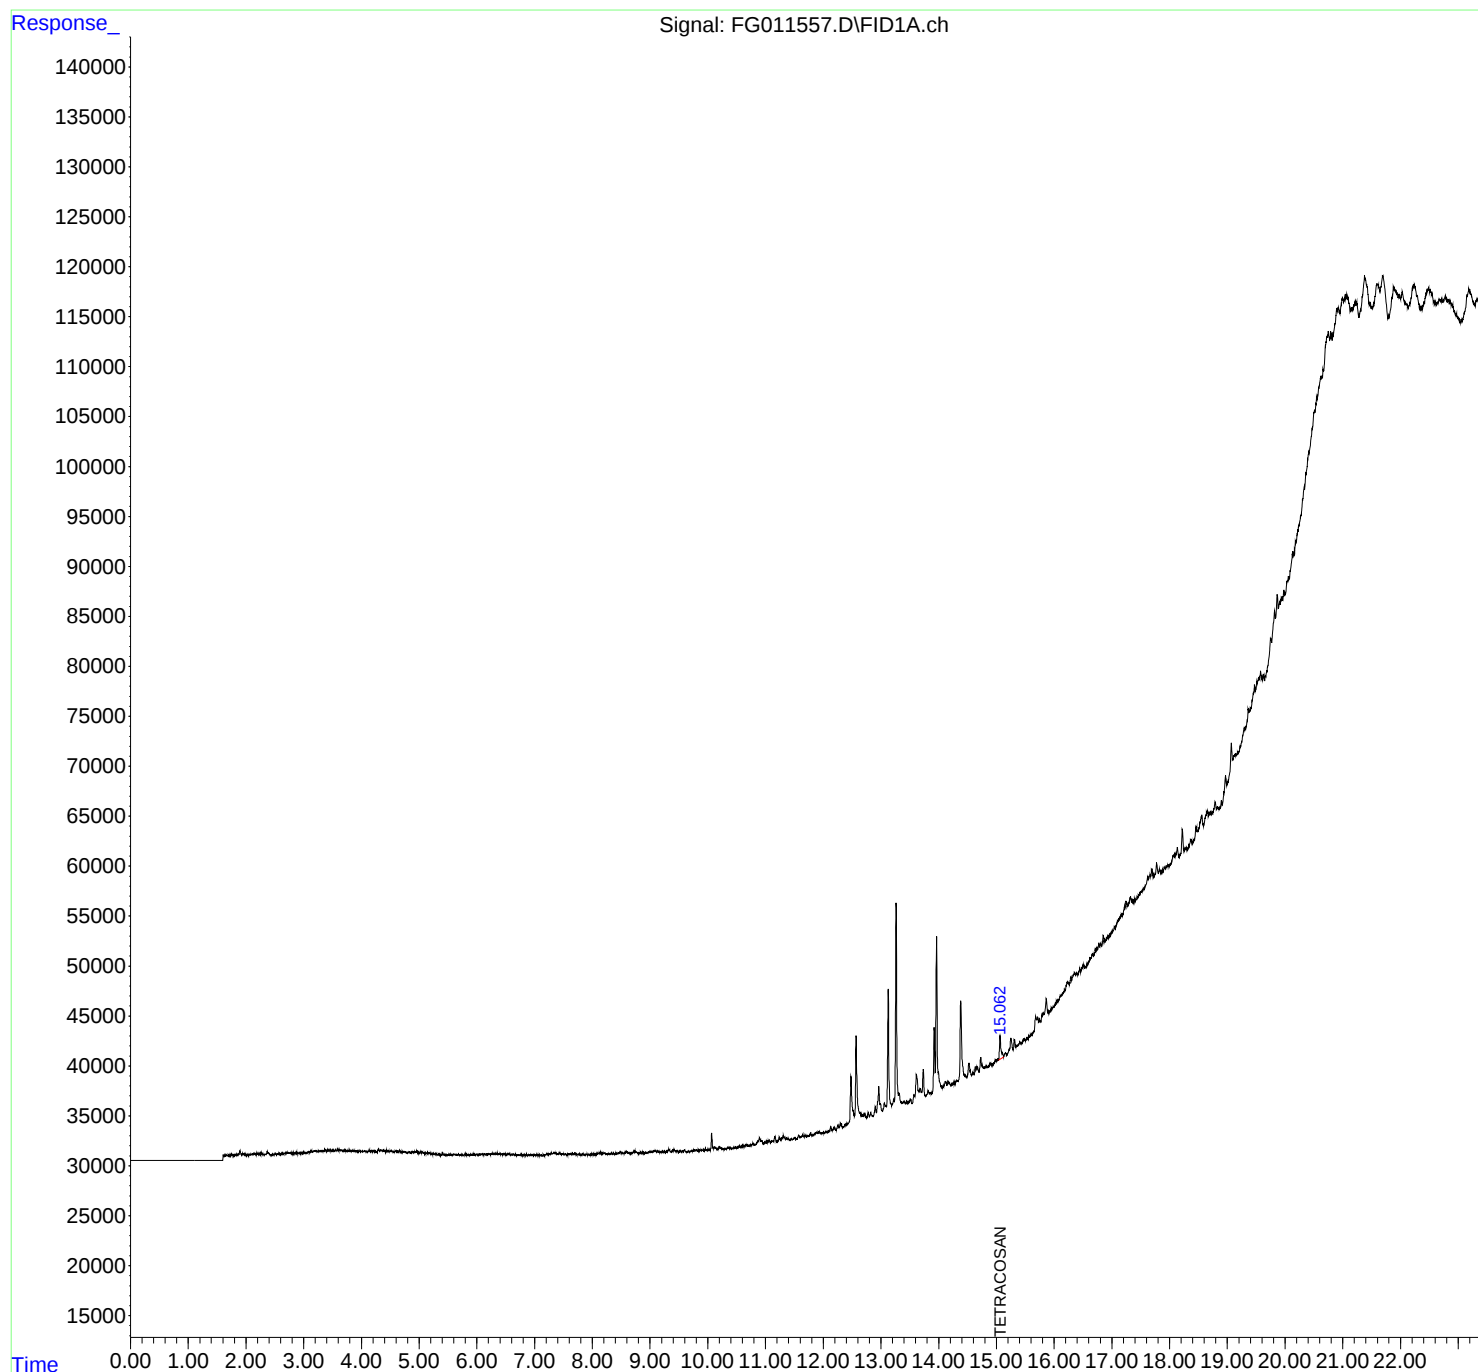

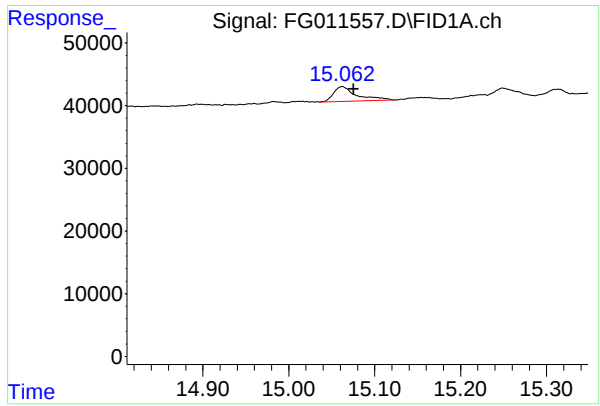

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.062 min
Delta R.T.: -0.013 min
Response: 44220
Conc: 0.42 ug/ml

Instrument :

FID_G

ClientSampleId :

SS-06-20230306

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 03/09/2023

Supervised By :Ankita Jodhani 03/10/2023