

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030923\
Data File : FG011561.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2023 12:53
Operator : YP\AJ
Sample : 01829-03 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SS-03-20230306

Integration File: autoint1.e
Quant Time: Mar 09 14:04:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.061	200083	1.902 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG030923\
Data File : FG011561.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2023 12:53
Operator : YP\AJ
Sample : 01829-03 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SS-03-20230306

Integration File: autoint1.e
Quant Time: Mar 09 14:04:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

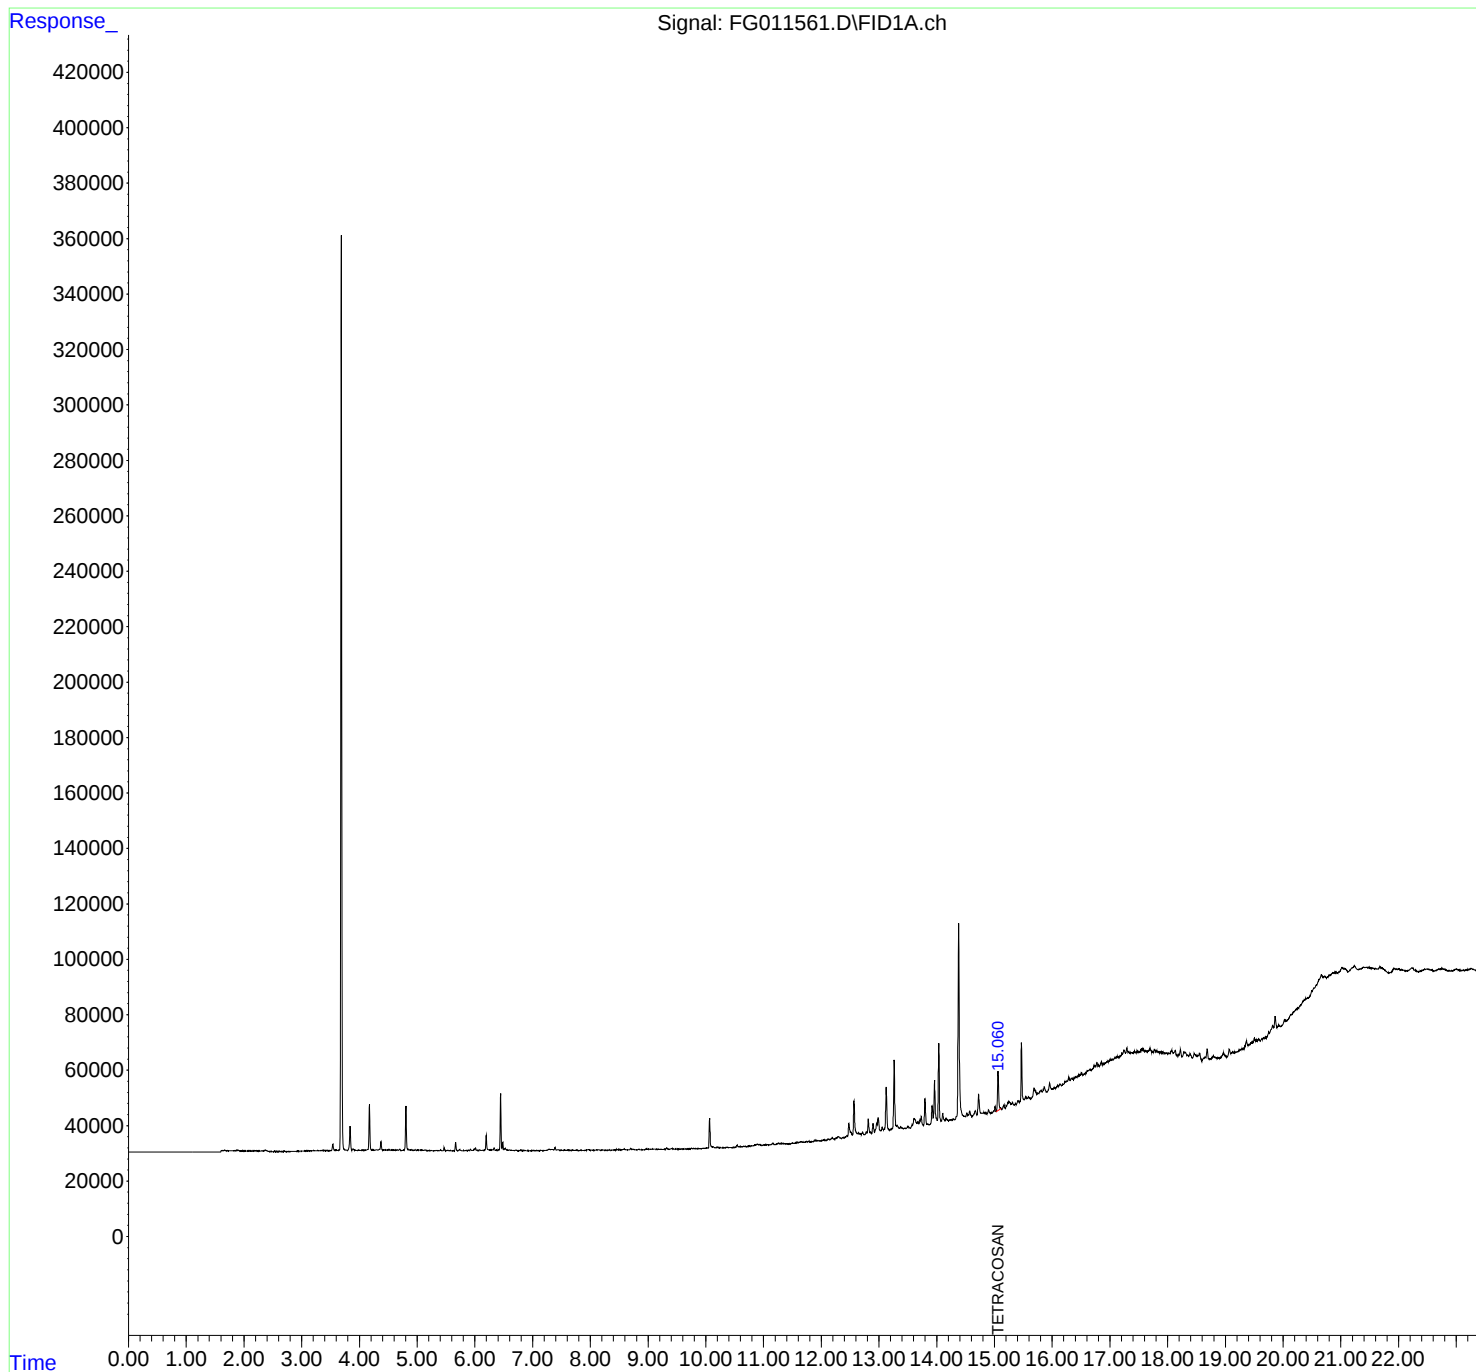

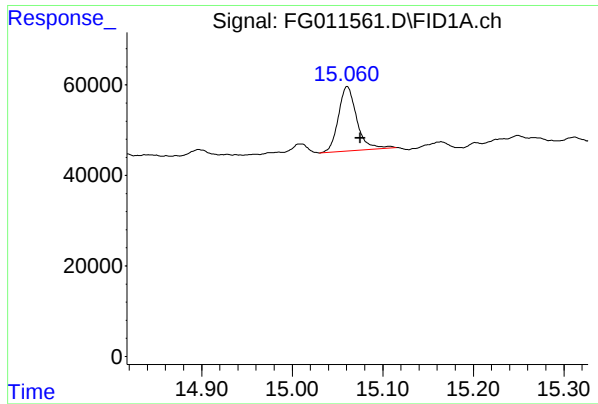

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.061 min
Delta R.T.: -0.015 min
Response: 200083
Conc: 1.90 ug/ml

Instrument :
FID_G
ClientSampleId :
SS-03-20230306