

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
 Data File : FG006785.D
 Signal(s) : FID1A.ch
 Acq On : 10 Mar 2020 17:51
 Operator : DD\AJ
 Sample : L1852-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 01:44:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.697	1540005	18.339 ug/ml
Target Compounds			
4) N-TETRADECANE	8.469	328928	3.621 ug/ml
10) N-TETRACOSANE	14.893	102921	1.068 ug/ml
11) N-HEXACOSANE	15.882	126115	1.340 ug/ml
12) N-OCTACOSANE	16.803	264688	2.818 ug/ml
13) N-TRIACONTANE	17.658	219508	2.339 ug/ml
14) N-DOTRIACONTANE	18.462	131124	1.504 ug/ml
16) N-HEXATRIACONTANE	19.931	165481	2.766 ug/ml
18) N-TETRACONTANE	21.387	219945	5.121 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
Data File : FG006785.D
Signal(s) : FID1A.ch
Acq On : 10 Mar 2020 17:51
Operator : DD\AJ
Sample : L1852-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 01:44:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

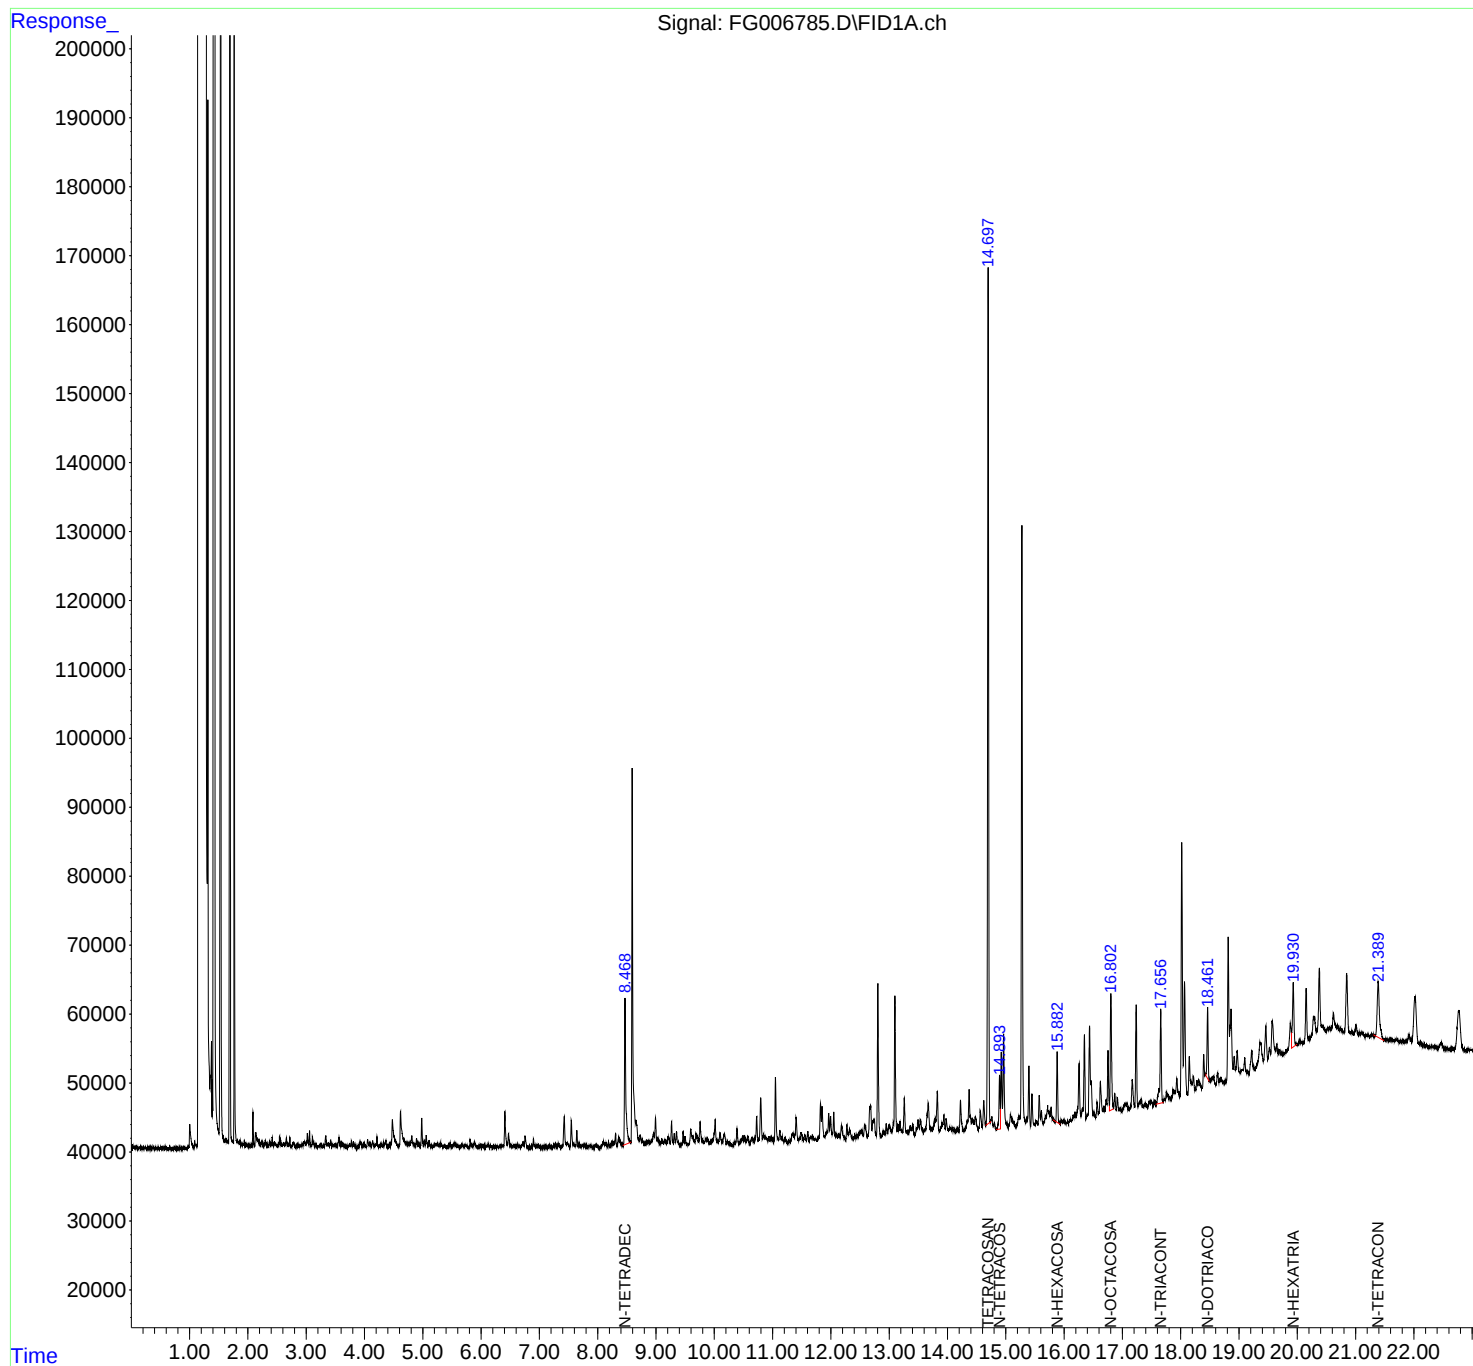


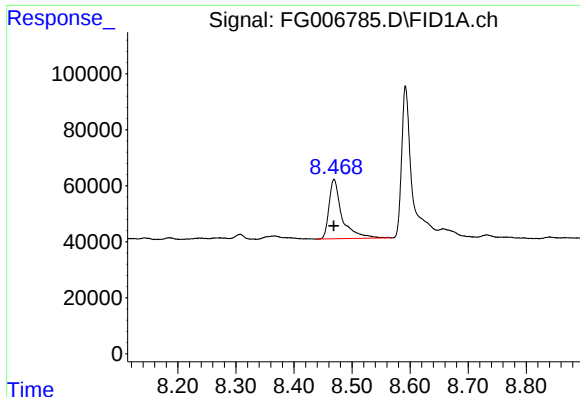

#4 N-TETRADECANE


R.T.: 8.469 min
Delta R.T.: 0.000 min
Response: 328928
Conc: 3.62 ug/ml

Instrument :
FID_G
ClientSampleId :

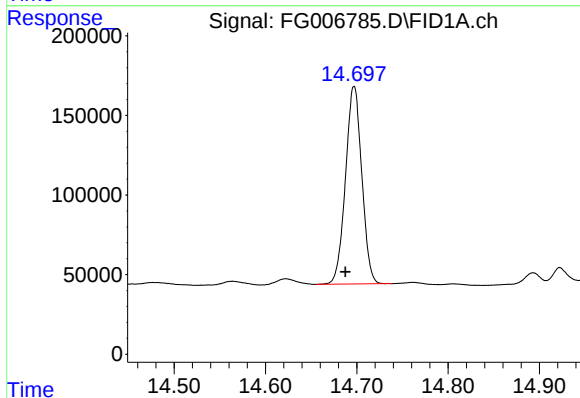


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.697 min
Delta R.T.: 0.009 min
Response: 1540005
Conc: 18.34 ug/ml

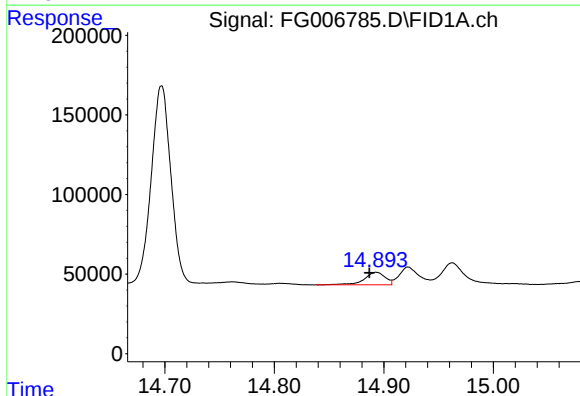


#10 N-TETRACOSANE

R.T.: 14.893 min
Delta R.T.: 0.006 min
Response: 102921
Conc: 1.07 ug/ml

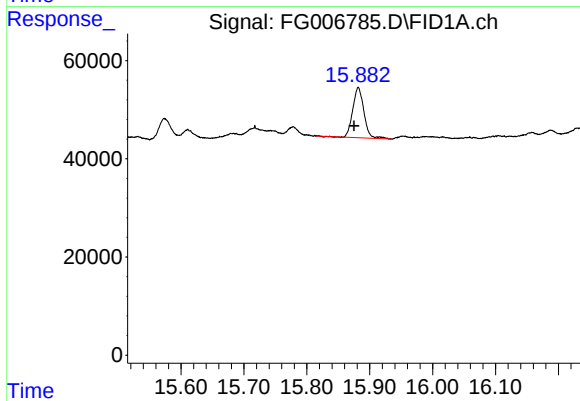

#11 N-HEXACOSANE


R.T.: 15.882 min
Delta R.T.: 0.007 min
Response: 126115
Conc: 1.34 ug/ml

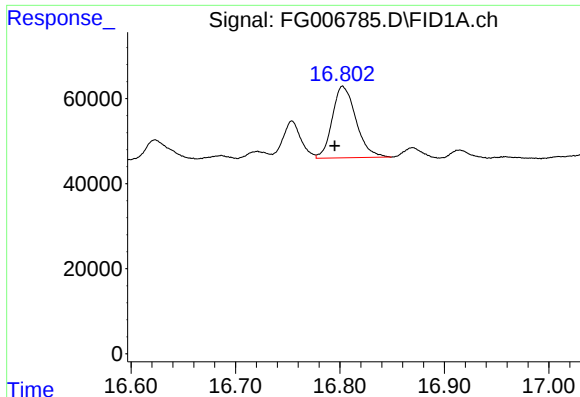

#12 N-OCTACOSANE


R.T.: 16.803 min
Delta R.T.: 0.008 min
Response: 264688
Conc: 2.82 ug/ml

Instrument :
FID_G
ClientSampleId :

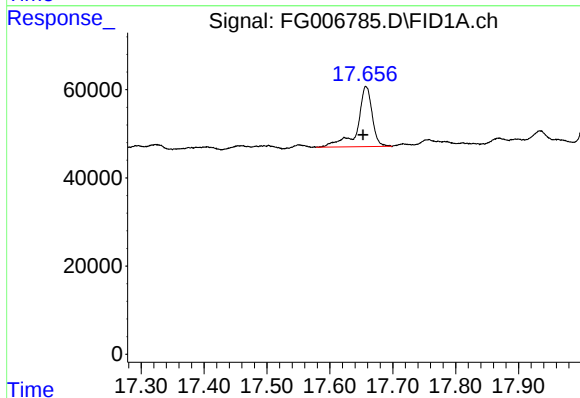


#13 N-TRIACONTANE

R.T.: 17.658 min
Delta R.T.: 0.005 min
Response: 219508
Conc: 2.34 ug/ml

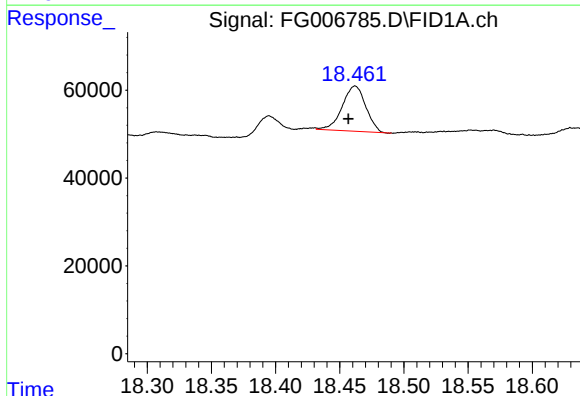


#14 N-DOTRIACONTANE

R.T.: 18.462 min
Delta R.T.: 0.005 min
Response: 131124
Conc: 1.50 ug/ml

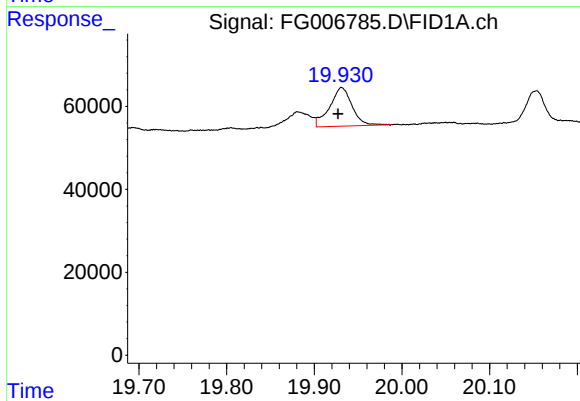

#16 N-HEXATRIACONTANE

R.T.: 19.931 min
Delta R.T.: 0.004 min
Response: 165481
Conc: 2.77 ug/ml

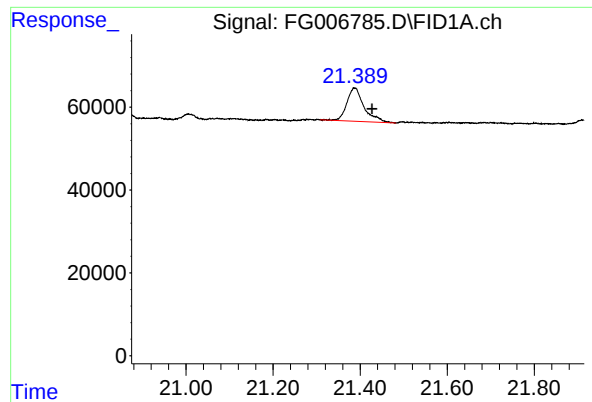

#18 N-TETRACONTANE

R.T.: 21.387 min
Delta R.T.: -0.040 min
Response: 219945
Conc: 5.12 ug/ml

Instrument :
FID_G
ClientSampleId :