

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
 Data File : FG006790.D
 Signal(s) : FID1A.ch
 Acq On : 10 Mar 2020 20:25
 Operator : DD\AJ
 Sample : L1852-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 01:45:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.699	1243484	14.808 ug/ml
Target Compounds			
7) N-EICOSANE	12.684	187531	1.899 ug/ml
8) N-DOCOSANE	13.824	163254	1.671 ug/ml
10) N-TETRACOSANE	14.921	684196	7.098 ug/ml
11) N-HEXACOSANE	15.885	218575	2.322 ug/ml
12) N-OCTACOSANE	16.810	901439	9.598 ug/ml
13) N-TRIACONTANE	17.662	436572	4.652 ug/ml
14) N-DOTRIACONTANE	18.460	408140	4.682 ug/ml
16) N-HEXATRIACONTANE	19.934	655108	10.952 ug/ml
18) N-TETRACONTANE	21.390	979208	22.797 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
Data File : FG006790.D
Signal(s) : FID1A.ch
Acq On : 10 Mar 2020 20:25
Operator : DD\AJ
Sample : L1852-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 01:45:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

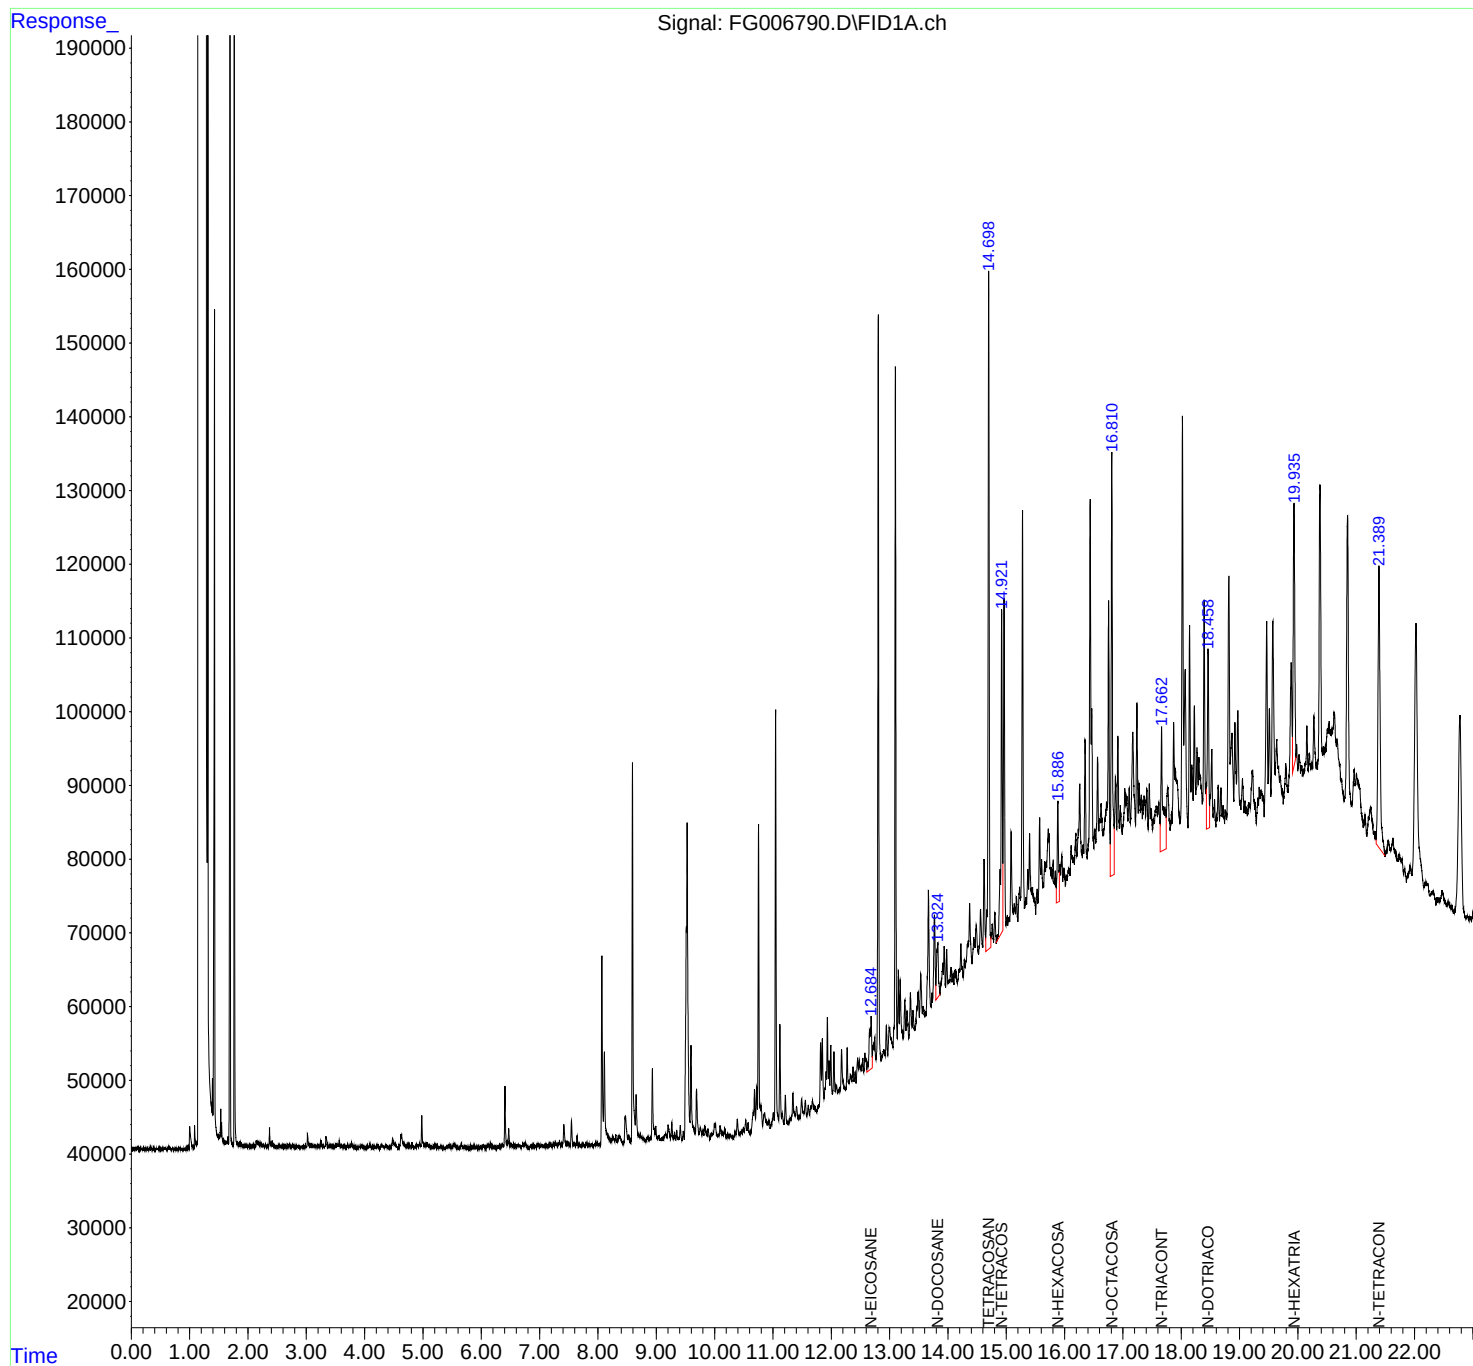


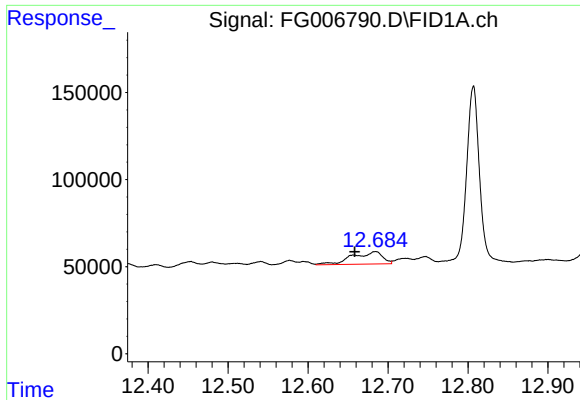

#7 N-EICOSANE


R.T.: 12.684 min
Delta R.T.: 0.026 min
Response: 187531
Conc: 1.90 ug/ml

Instrument :
FID_G
ClientSampleId :

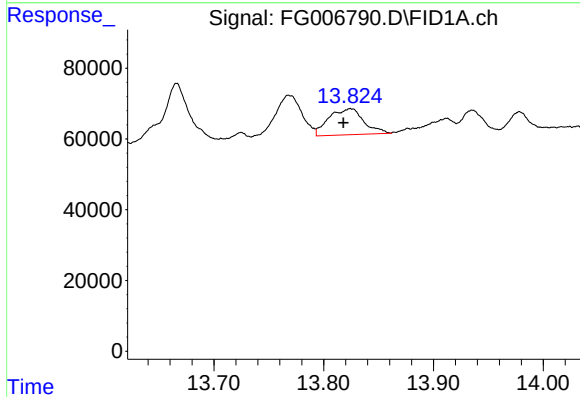


#8 N-DOCOSANE

R.T.: 13.824 min
Delta R.T.: 0.006 min
Response: 163254
Conc: 1.67 ug/ml

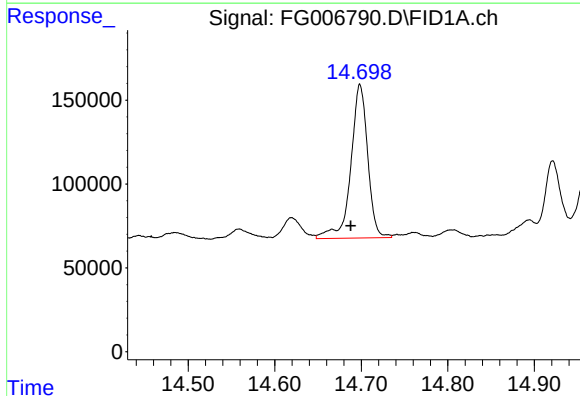


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.699 min
Delta R.T.: 0.011 min
Response: 1243484
Conc: 14.81 ug/ml

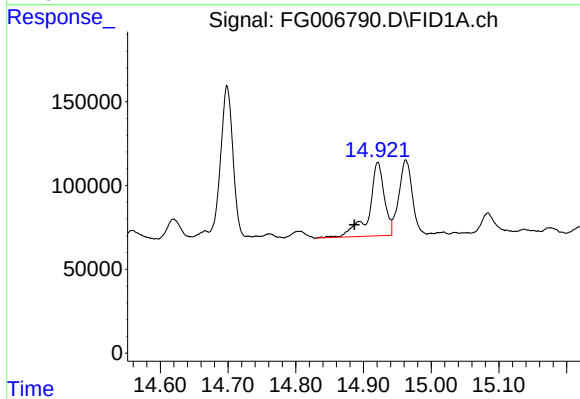

#10 N-TETRACOSANE


R.T.: 14.921 min
Delta R.T.: 0.035 min
Response: 684196
Conc: 7.10 ug/ml

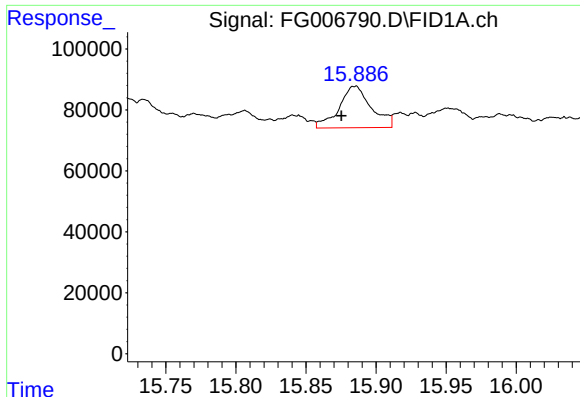

#11 N-HEXACOSANE


R.T.: 15.885 min
Delta R.T.: 0.010 min
Response: 218575
Conc: 2.32 ug/ml

Instrument :
FID_G
ClientSampleId :

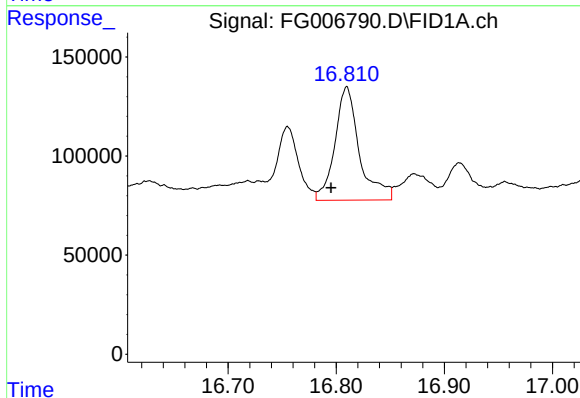


#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: 0.014 min
Response: 901439
Conc: 9.60 ug/ml

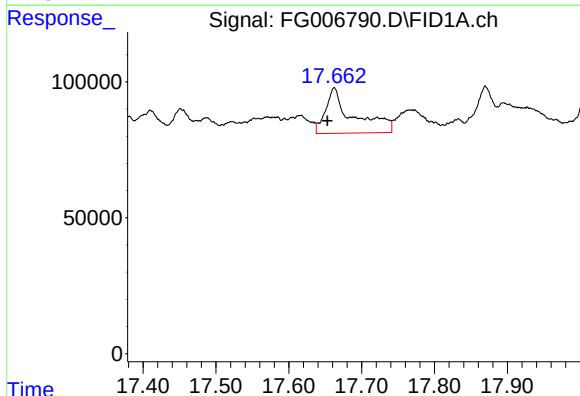


#13 N-TRIACONTANE

R.T.: 17.662 min
Delta R.T.: 0.009 min
Response: 436572
Conc: 4.65 ug/ml

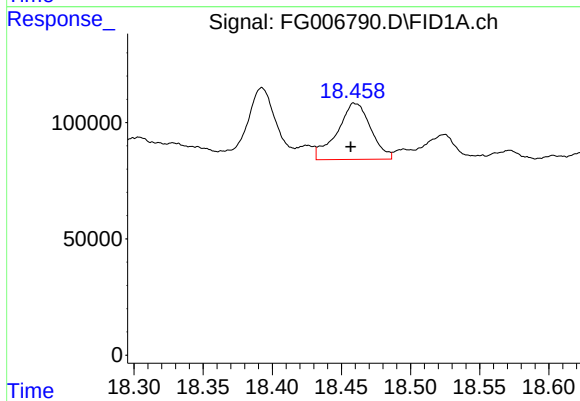

#14 N-DOTRIACONTANE


R.T.: 18.460 min
Delta R.T.: 0.003 min
Response: 408140
Conc: 4.68 ug/ml

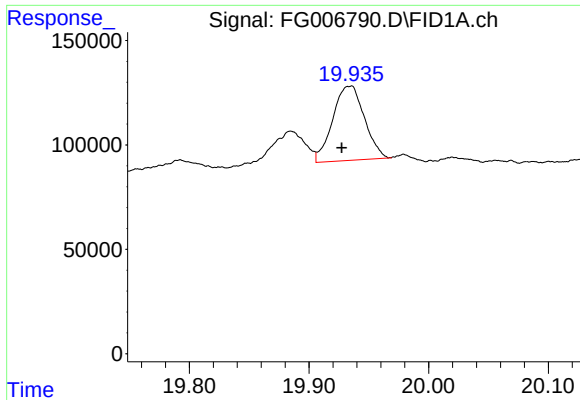

#16 N-HEXATRIACONTANE

R.T.: 19.934 min
Delta R.T.: 0.006 min
Response: 655108
Conc: 10.95 ug/ml

Instrument :
FID_G
ClientSampleId :

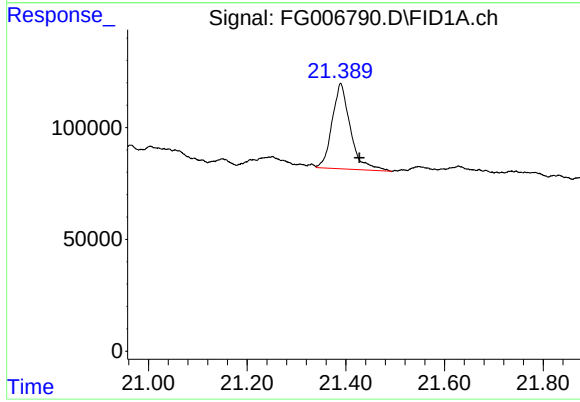

#18 N-TETRACONTANE

R.T.: 21.390 min
Delta R.T.: -0.038 min
Response: 979208
Conc: 22.80 ug/ml