

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
 Data File : FG006794.D
 Signal(s) : FID1A.ch
 Acq On : 10 Mar 2020 22:28
 Operator : DD\AJ
 Sample : L1852-02 2X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 01:45:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.697	936694	11.155 ug/ml
Target Compounds			
6) N-OCTADECANE	11.341f	116722	1.184 ug/ml
7) N-EICOSANE	12.686	100624	1.019 ug/ml
8) N-DOCOSANE	13.810	143103	1.465 ug/ml
10) N-TETRACOSANE	14.921	854081	8.860 ug/ml
12) N-OCTACOSANE	16.809	750246	7.988 ug/ml
13) N-TRIACONTANE	17.661	174867	1.863 ug/ml
14) N-DOTRIACONTANE	18.464	242080	2.777 ug/ml
16) N-HEXATRIACONTANE	19.940	103245	1.726 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
Data File : FG006794.D
Signal(s) : FID1A.ch
Acq On : 10 Mar 2020 22:28
Operator : DD\AJ
Sample : L1852-02 2X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 01:45:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

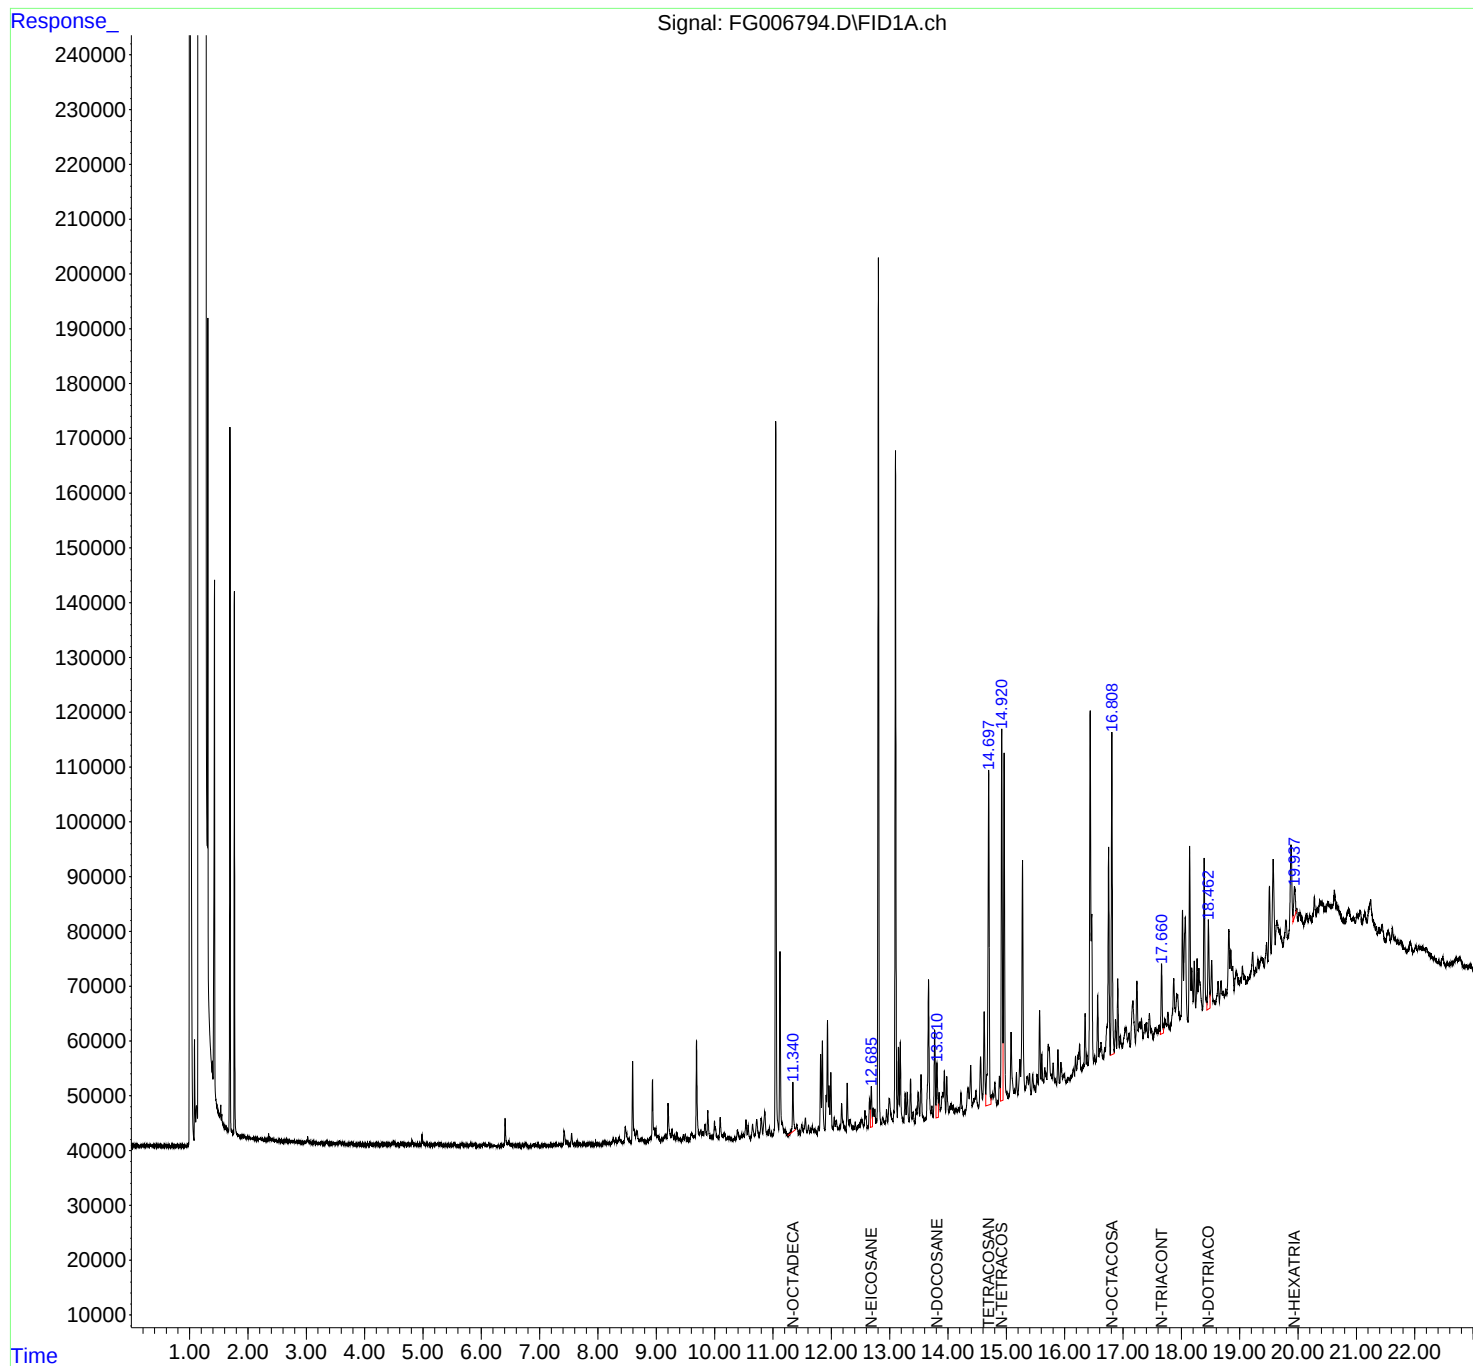


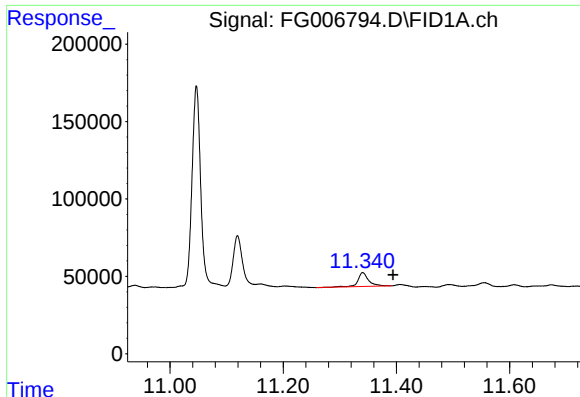

#6 N-OCTADECANE


R.T.: 11.341 min
Delta R.T.: -0.054 min
Response: 116722
Conc: 1.18 ug/ml

Instrument :
FID_G
ClientSampleId :

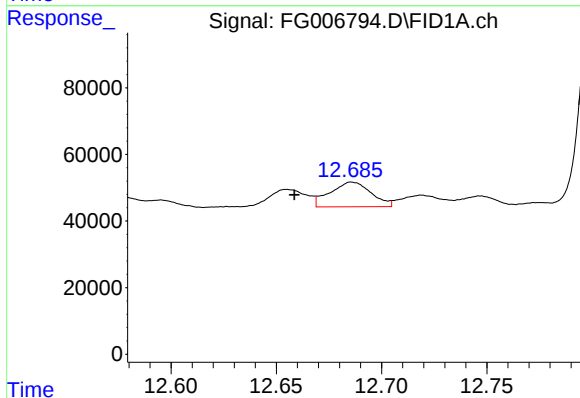


#7 N-EICOSANE

R.T.: 12.686 min
Delta R.T.: 0.028 min
Response: 100624
Conc: 1.02 ug/ml

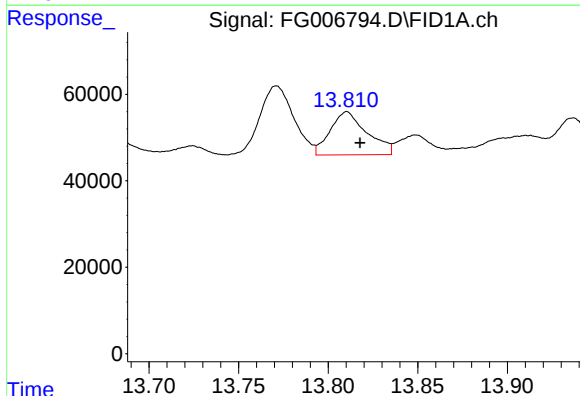


#8 N-DOCOSANE

R.T.: 13.810 min
Delta R.T.: -0.007 min
Response: 143103
Conc: 1.46 ug/ml

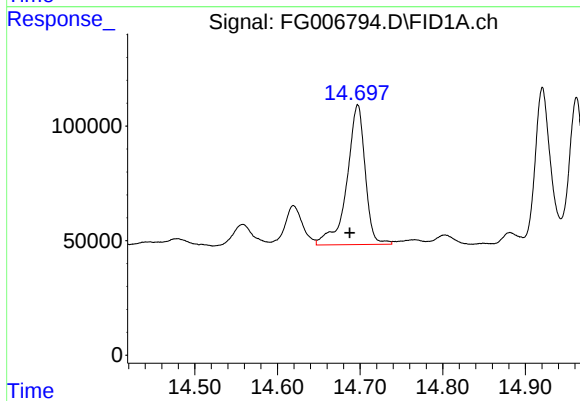

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.697 min
Delta R.T.: 0.009 min
Response: 936694
Conc: 11.15 ug/ml

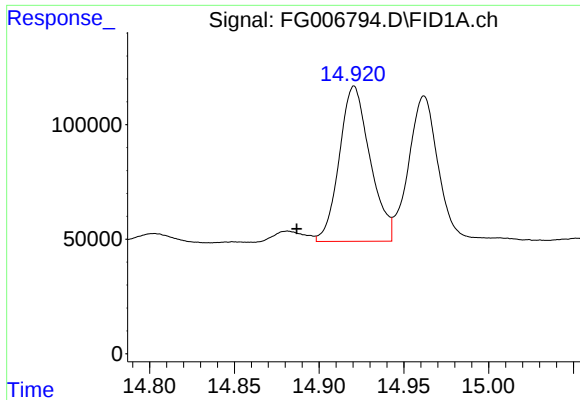

#10 N-TETRACOSANE


R.T.: 14.921 min
Delta R.T.: 0.034 min
Response: 854081
Conc: 8.86 ug/ml

Instrument :
FID_G
ClientSampleId :

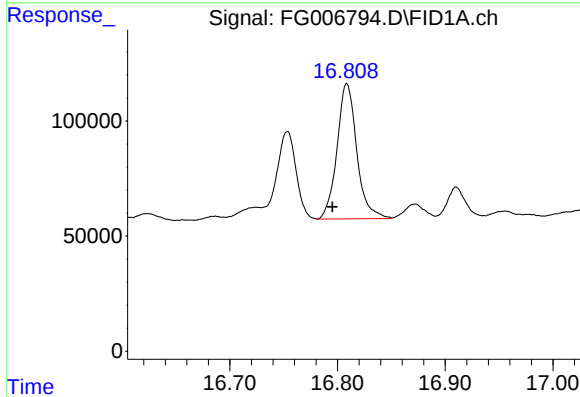


#12 N-OCTACOSANE

R.T.: 16.809 min
Delta R.T.: 0.014 min
Response: 750246
Conc: 7.99 ug/ml

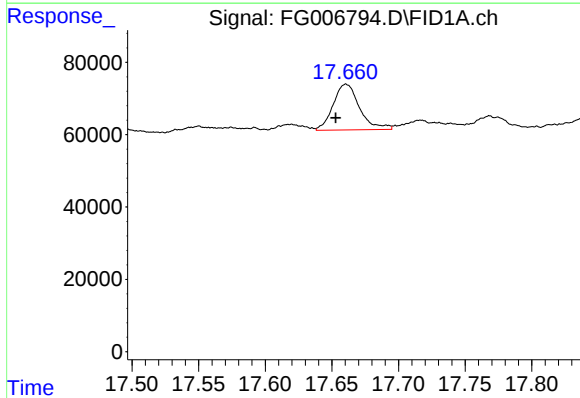


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: 0.008 min
Response: 174867
Conc: 1.86 ug/ml

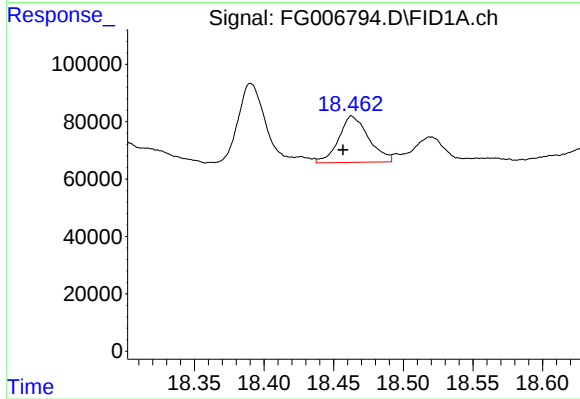

#14 N-DOTRIACONTANE

R.T.: 18.464 min
Delta R.T.: 0.007 min
Response: 242080
Conc: 2.78 ug/ml

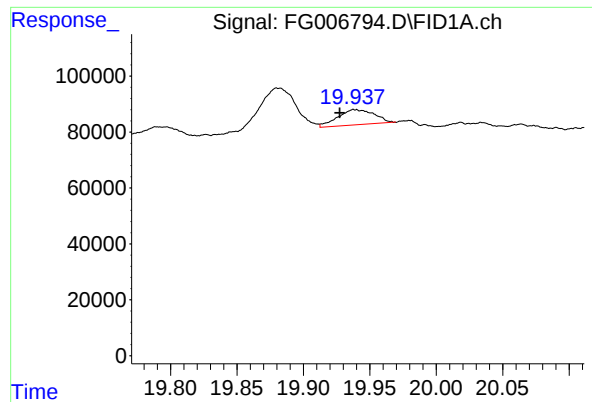

#16 N-HEXATRIACONTANE

R.T.: 19.940 min
Delta R.T.: 0.012 min
Response: 103245
Conc: 1.73 ug/ml

Instrument :
FID_G
ClientSampleId :