

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
 Data File : FG006798.D
 Signal(s) : FID1A.ch
 Acq On : 11 Mar 2020 00:31
 Operator : DD\AJ
 Sample : L1852-06 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 01:46:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.698	173795	2.070 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.924	284347	2.950 ug/ml
12) N-OCTACOSANE	16.812	309855	3.299 ug/ml
14) N-DOTRIACONTANE	18.394f	206029	2.364 ug/ml
16) N-HEXATRIACONTANE	19.884	193447	3.234 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
Data File : FG006798.D
Signal(s) : FID1A.ch
Acq On : 11 Mar 2020 00:31
Operator : DD\AJ
Sample : L1852-06 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 01:46:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

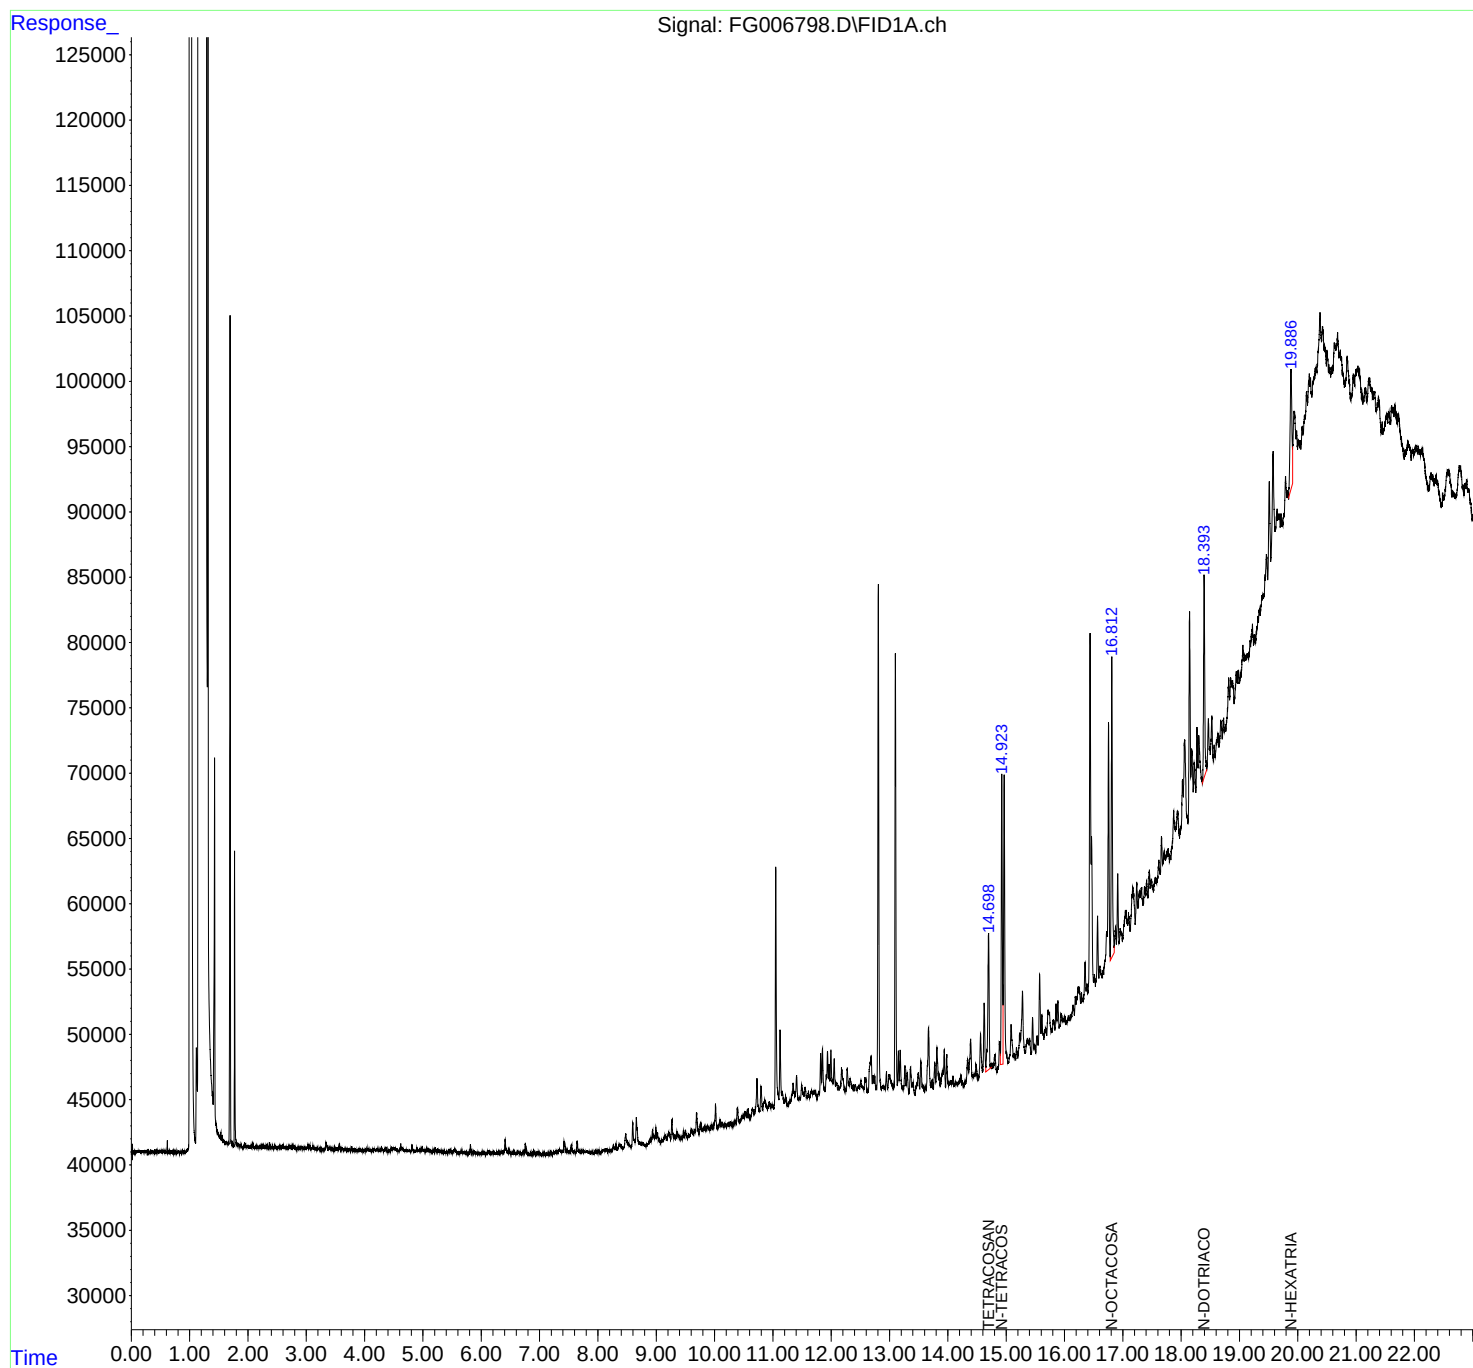


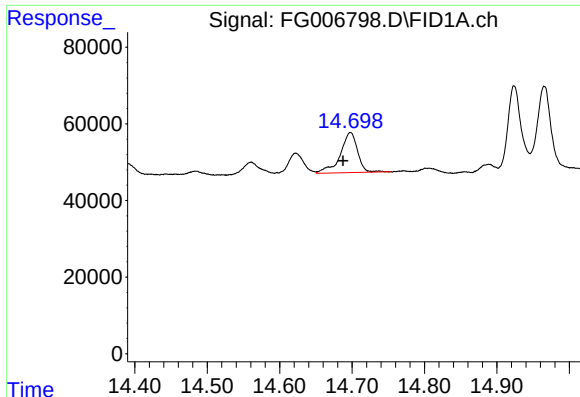

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.698 min
Delta R.T.: 0.010 min
Response: 173795
Conc: 2.07 ug/ml

Instrument :
FID_G
ClientSampleId :

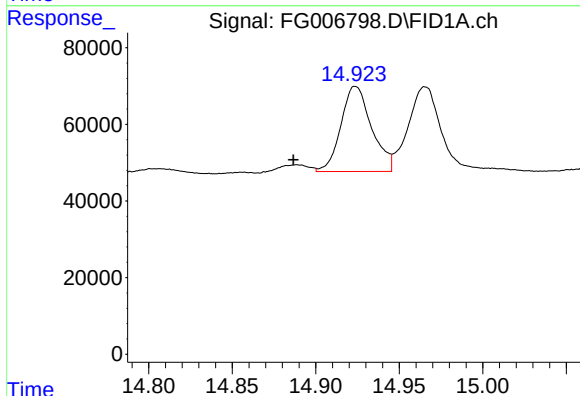


#10 N-TETRACOSANE

R.T.: 14.924 min
Delta R.T.: 0.037 min
Response: 284347
Conc: 2.95 ug/ml

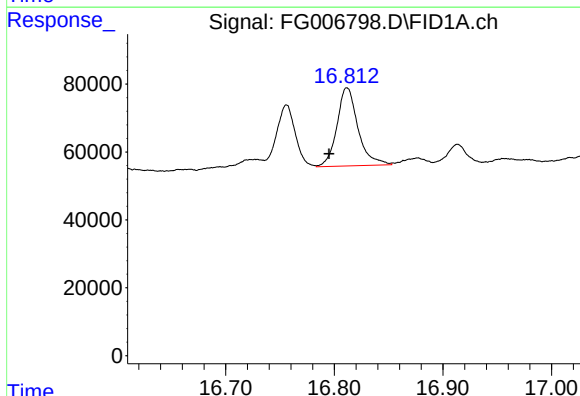


#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: 0.017 min
Response: 309855
Conc: 3.30 ug/ml

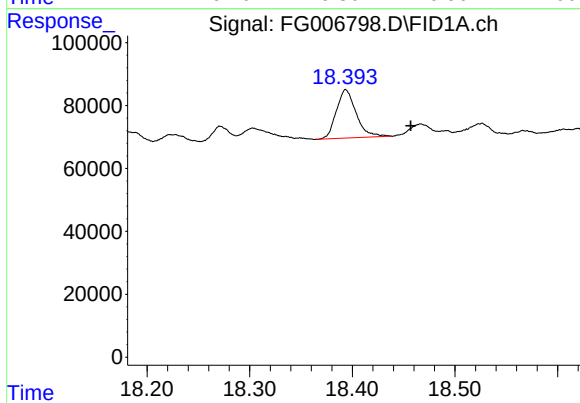

#14 N-DOTRIACONTANE

R.T.: 18.394 min
Delta R.T.: -0.063 min
Response: 206029
Conc: 2.36 ug/ml

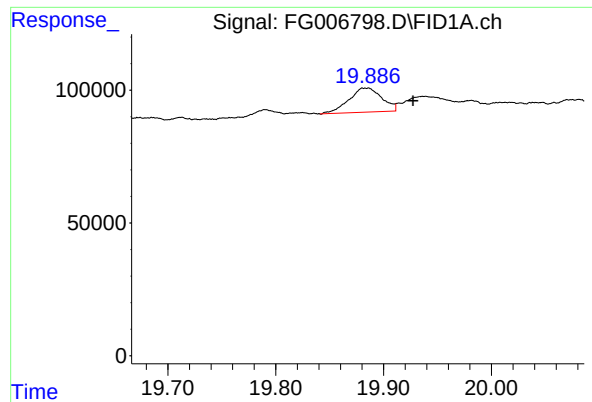

#16 N-HEXATRIACONTANE

R.T.: 19.884 min
Delta R.T.: -0.044 min
Response: 193447
Conc: 3.23 ug/ml

Instrument :
FID_G
ClientSampleId :